

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](#)

Operator:



Laboratory and Equipment

Laboratory Owner and Location
Goniospectrometer System and Type
Sensor Name, Calibr. Date and Serial No.
Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark
LabSpion – Type C, horizontal
LabSensor Model2 – 11-1-2024 – 3130191315
Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

Measurement Conditions

Number of C-planes and Resolution
 γ (gamma)-Resolution
Test Distance
Input Power, Power and Displ. Factors
Input RMS Voltage and Current
Frequency of Input Power
Warm-up Time and Variation

12 planes – 30°
5°
4,79 m
16,1 W – PF 0,96 – DPF 0,97
230 V – 0,073 A
50 Hz
Lamp stabilized in 15 min 1 sec – 2,0%

Tested Light Source



Product Name
Item No. and Manufacturer
Product Description (line 1)

803209-3000K-16W
803209-3000K-16W – Dutchfulfillment
3-FASE RAILARMATUUR | TARVOS | 60CM | WIT | CCT SWITCH

Main Light Measurement Results

Output – Total Lumen (Up% / Down%)
Efficiency
Peak Intensity and Beam Angle
Correlated Color Temperature, Target/Measured
Color Rendering Index
Color Rendering TM30-18
Color Shift, CIE duv and MacAdam Steps
Flicker

2245 lm – 3,96% / 96,04%
139 lm/W
896 cd – 97,1°
CCT = 3000 K / 3123 K
CRI 81,2
 R_f 81,8 – R_g 98,8
Duv 0,0015 – SDCM 4,2
SVM 0,03 – PstLM 0,1

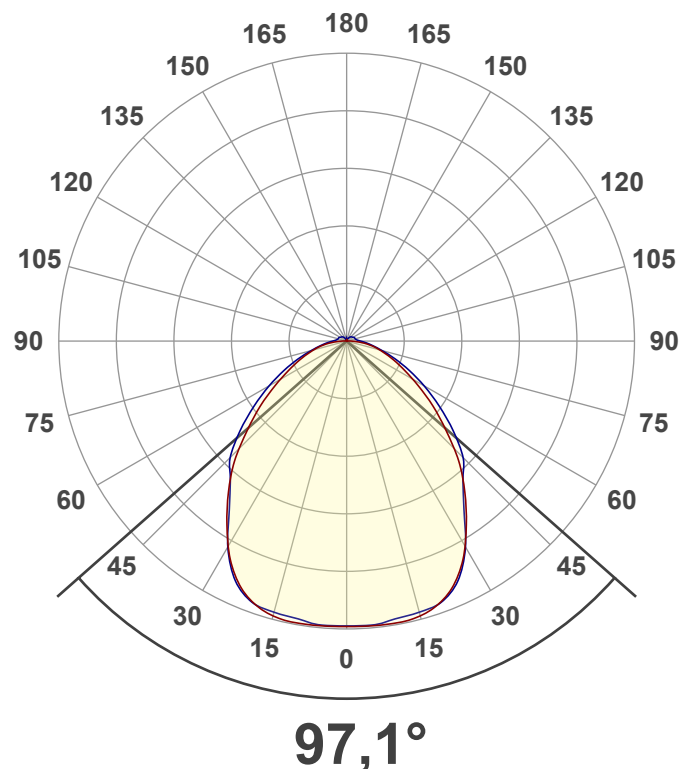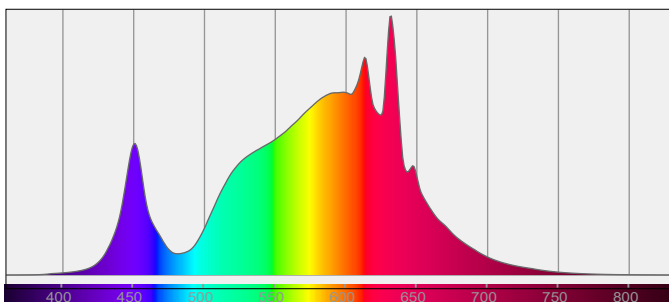

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS


Measurement tracking No. and Link: [VT250514-005869](#)

Operator:



Luminous Intensity diagram

Unit: 0-100% of peak intensity

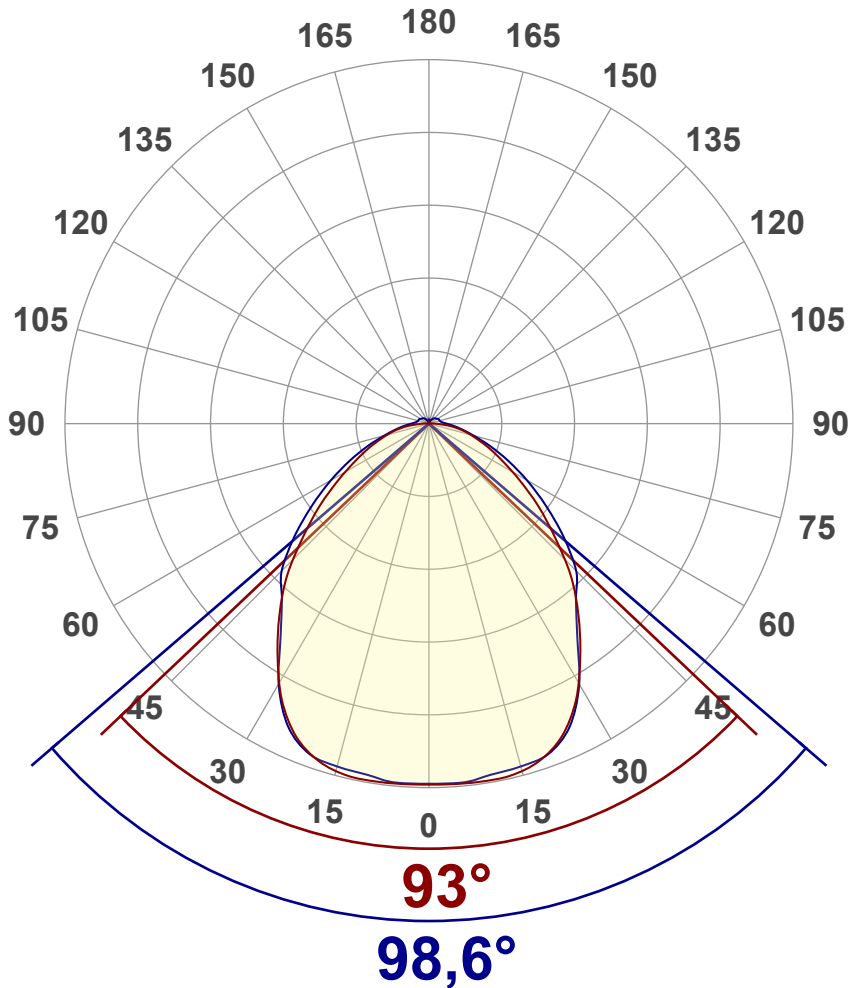

Main Values

Output (total Lumen)	2245 lm
Lumen Up% / Down%	3,96% / 96,04%
Peak Intensity	896 cd
Beam Angle (50%)	97,1°
Beam Angle (90%)	98,6°
Beam Angle (10%)	93°

Cut-off Angle

Average 2,5%	208,5°
--------------	--------

Field Angle

Average 10%	156°
-------------	------


Intensity Ratio

In 120° cone	79,3%
In 90° cone	57,6%

C000-C180

C090-C270

Linear distribution diagram - Intensity (candela) vs γ -angle

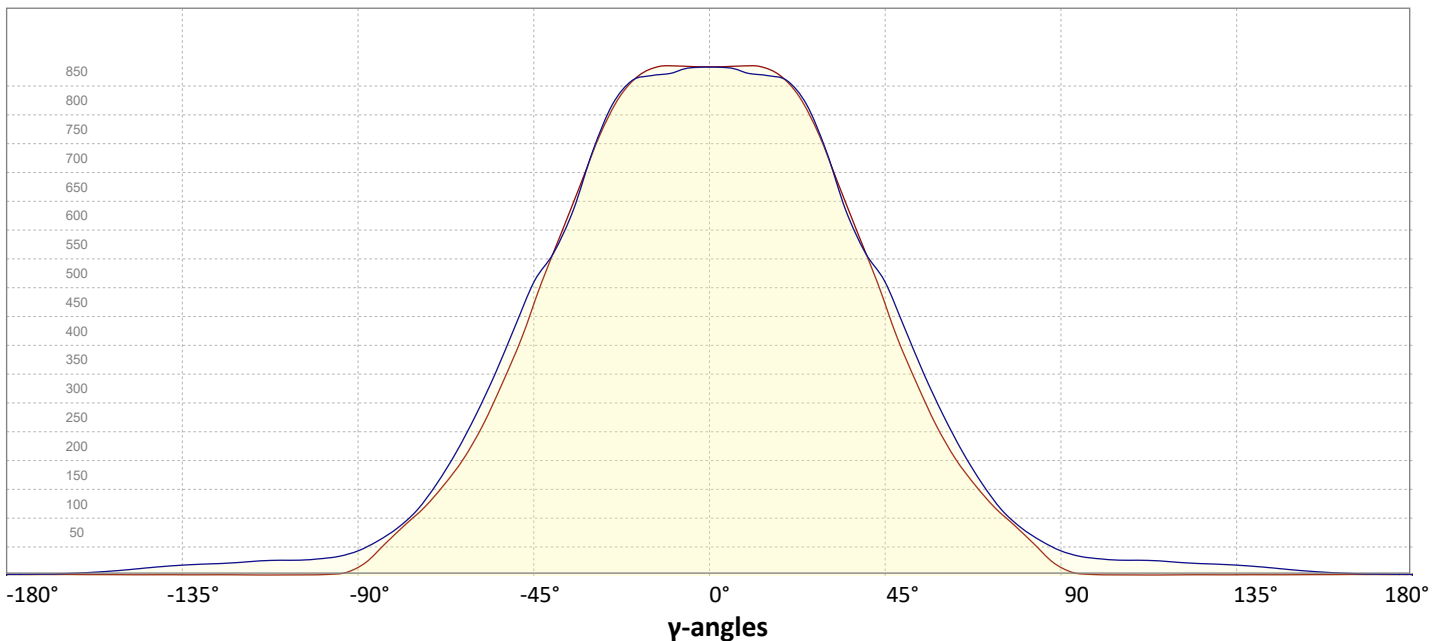

Light Measurement Report

Print date: 14-5-2025


Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](#)

Operator:




Iso-intensity Diagram (Iso-candela)

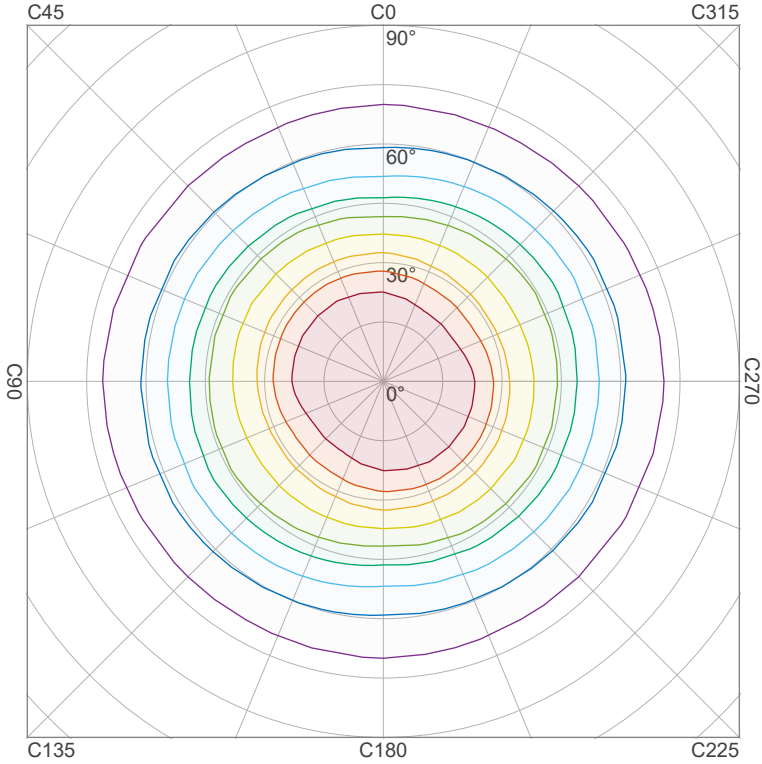

90 %	804,6 cd
80 %	715,2 cd
70 %	625,8 cd
60 %	536,4 cd
50 %	447,0 cd
40 %	357,6 cd
30 %	268,2 cd
20 %	178,8 cd
10 %	89,4 cd

Peak intensity: 894,0 cd
Number of c-planes: 12

Iso-illuminance Diagram (Iso-lux)

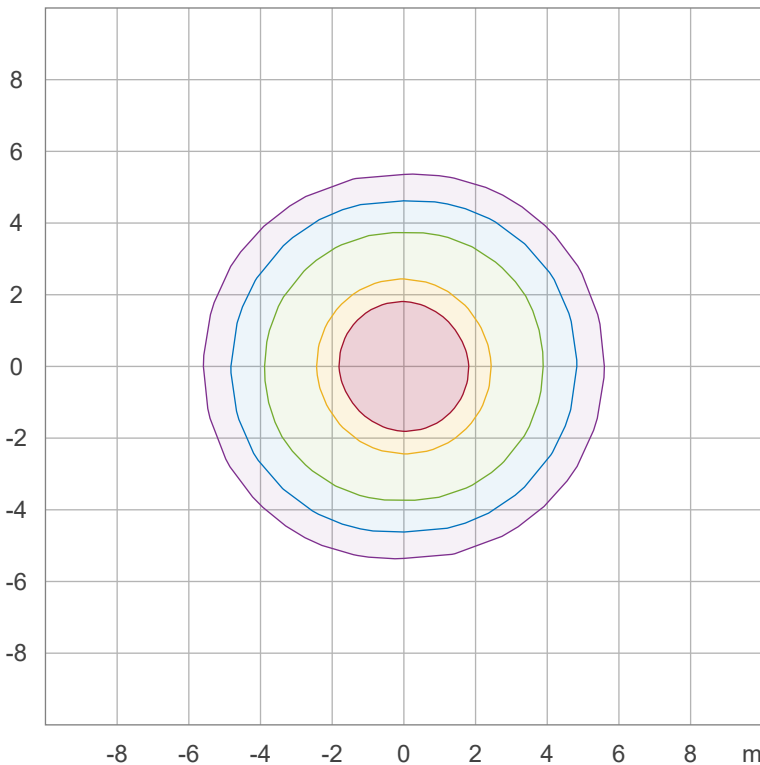

50,0 %	49,6 lx
30,0 %	29,8 lx
10,0 %	9,9 lx
5,0 %	5,0 lx
3,0 %	3,0 lx

Peak illuminance: 99,3 lx
Mounting height: 3,0 m
Number of c-planes: 12

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](https://www.viso-systems.com/VT250514-005869)

Operator:



Color details

Correlated Color Temperature, Target CCT = 3000 K
 Correlated Color Temperature, Measured CCT = 3123 K
 Color Rendering Index CRI 81,2
 Color Rendering Index, R9 (red component) R9 = 12,9
 Color Rendering TM30-18 R_f 81,8 – R_g 98,8
 Color Quality Scale CQS = 80,1

MacAdam Steps SDCM = 4,2
 Color coordinates CIE 1931 (x;y) = (0,437;0,404)
 Color coordinate CIEs 1960 (u;v) = (0,251;0,348)
 Color deviation from BBL Duv = 0,0015
 Color coordinate CIEs 1976 (CIELUV) (u';v') = (0,251;0,521)


CIE 1931



CIE 1931 – zoomed on Planckian locus




Color Rendering Index per reference color (CIE 1995)

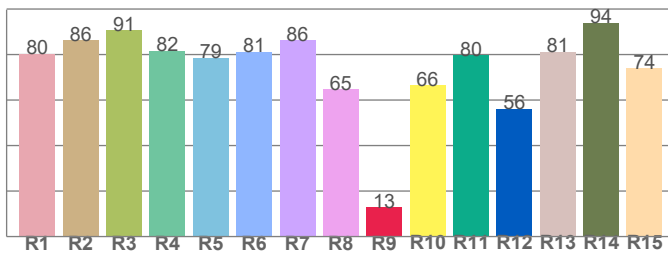


CRI R values, only R1-R8 are used to calculate final CRI value

R1	R2	R3	R4	R5	R6	R7	R8	R9	R10	R11	R12	R13	R14	R15
80,4	86,2	90,6	81,6	78,7	81,3	86,1	64,7	12,9	66,4	79,8	56,1	81,1	93,9	73,9

Spectral power distribution (SPD) / W/nm – 0-100%

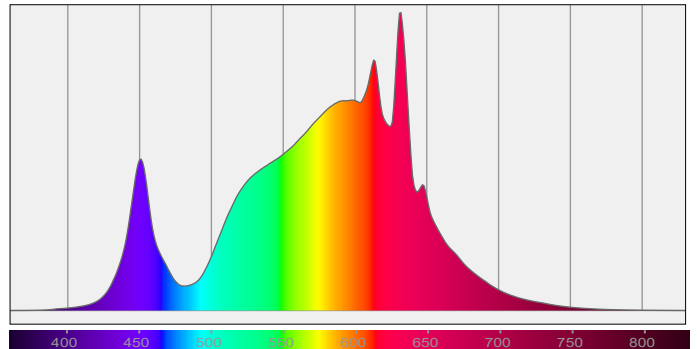


TM30-18 R_f-values per hue bin

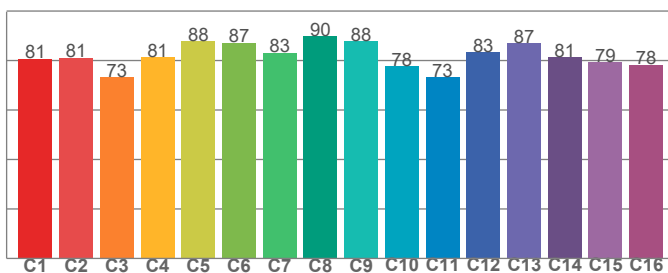

TM30 C values, 16 binned values out of total of 99 C values

C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
80,7	81,1	73,1	81,4	87,7	87,2	83,2	89,8	87,9	77,7	73,3	83,5	87,0	81,4	79,3	78,2

Color Quality Scale by reference color

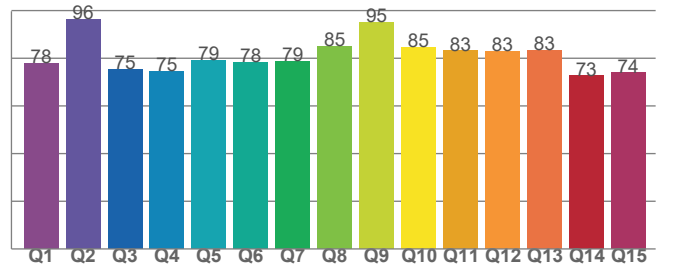

CQS Q values

Q1	Q2	Q3	Q4	Q5	Q6	Q7	Q8	Q9	Q10	Q11	Q12	Q13	Q14	Q15
77,9	96,4	75,3	74,5	79,3	78,4	78,8	85,0	95,0	84,6	83,1	82,9	83,3	72,6	74,0

Light Measurement Report

Print date: 14-5-2025


Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](https://www.viso-systems.com/VT250514-005869)

Operator:



Beam Details

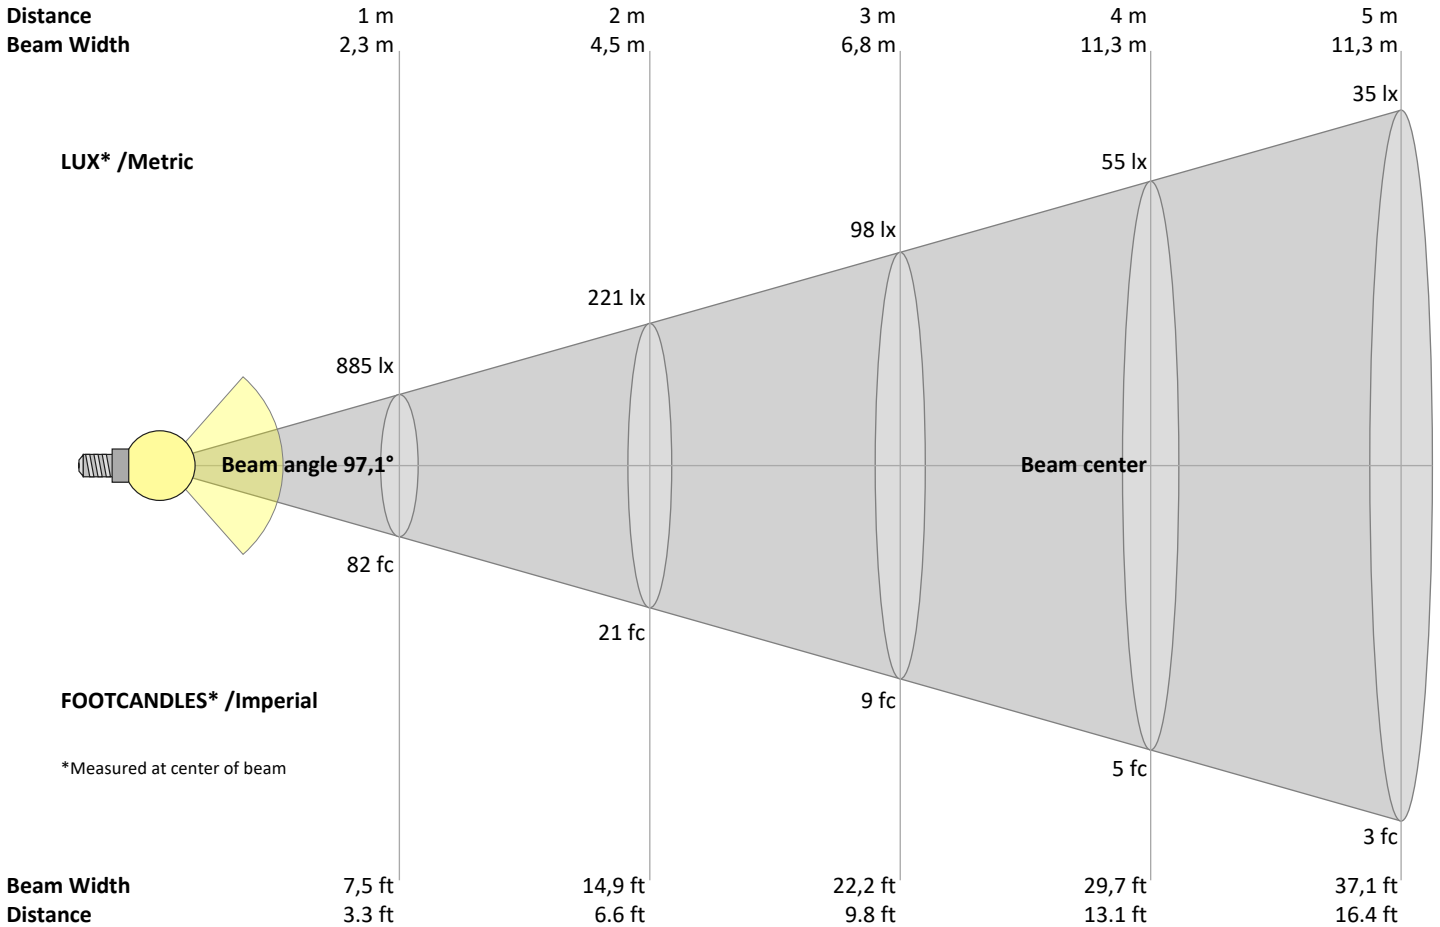

Beam intensities from 1 – 20 m

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	m
3,3	6,6	9,8	13,1	16,4	19,7	23	26,2	29,5	32,8	36,1	39,4	42,7	45,9	49,2	52,5	55,8	59,1	62,3	65,6	ft
885	221	98	55	35	25	18	14	11	9	7	6	5	5	4	3	3	3	2	2	lux
82,2	20,6	9,1	5,1	3,3	2,3	1,7	1,3	1	0,8	0,7	0,6	0,5	0,4	0,4	0,3	0,3	0,3	0,2	0,2	fc

Intensities in 0° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
885	884	884	878	854	805	731	645	560	471	382	306	238	185	142	106	75	43	16	4	cd
100%	100%	100%	99%	96%	91%	83%	73%	63%	53%	43%	35%	27%	21%	16%	12%	8%	5%	2%	0%	of 0°val

Intensities in 90° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
885	881	872	868	858	816	735	633	560	509	429	349	277	213	158	113	82	60	43	34	cd
100%	100%	99%	98%	97%	92%	83%	71%	63%	57%	49%	39%	31%	24%	18%	13%	9%	7%	5%	4%	of 0°val

Intensities in 180° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
885	884	884	878	854	805	731	645	560	471	382	306	238	185	142	106	75	43	16	4	cd
100%	100%	100%	99%	96%	91%	83%	73%	63%	53%	43%	35%	27%	21%	16%	12%	8%	5%	2%	0%	of 0°val

Intensities in 270° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
885	881	872	868	858	816	735	633	560	509	429	349	277	213	158	113	82	60	43	34	cd
100%	100%	99%	98%	97%	92%	83%	71%	63%	57%	49%	39%	31%	24%	18%	13%	9%	7%	5%	4%	of 0°val

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](#)


Operator:



Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

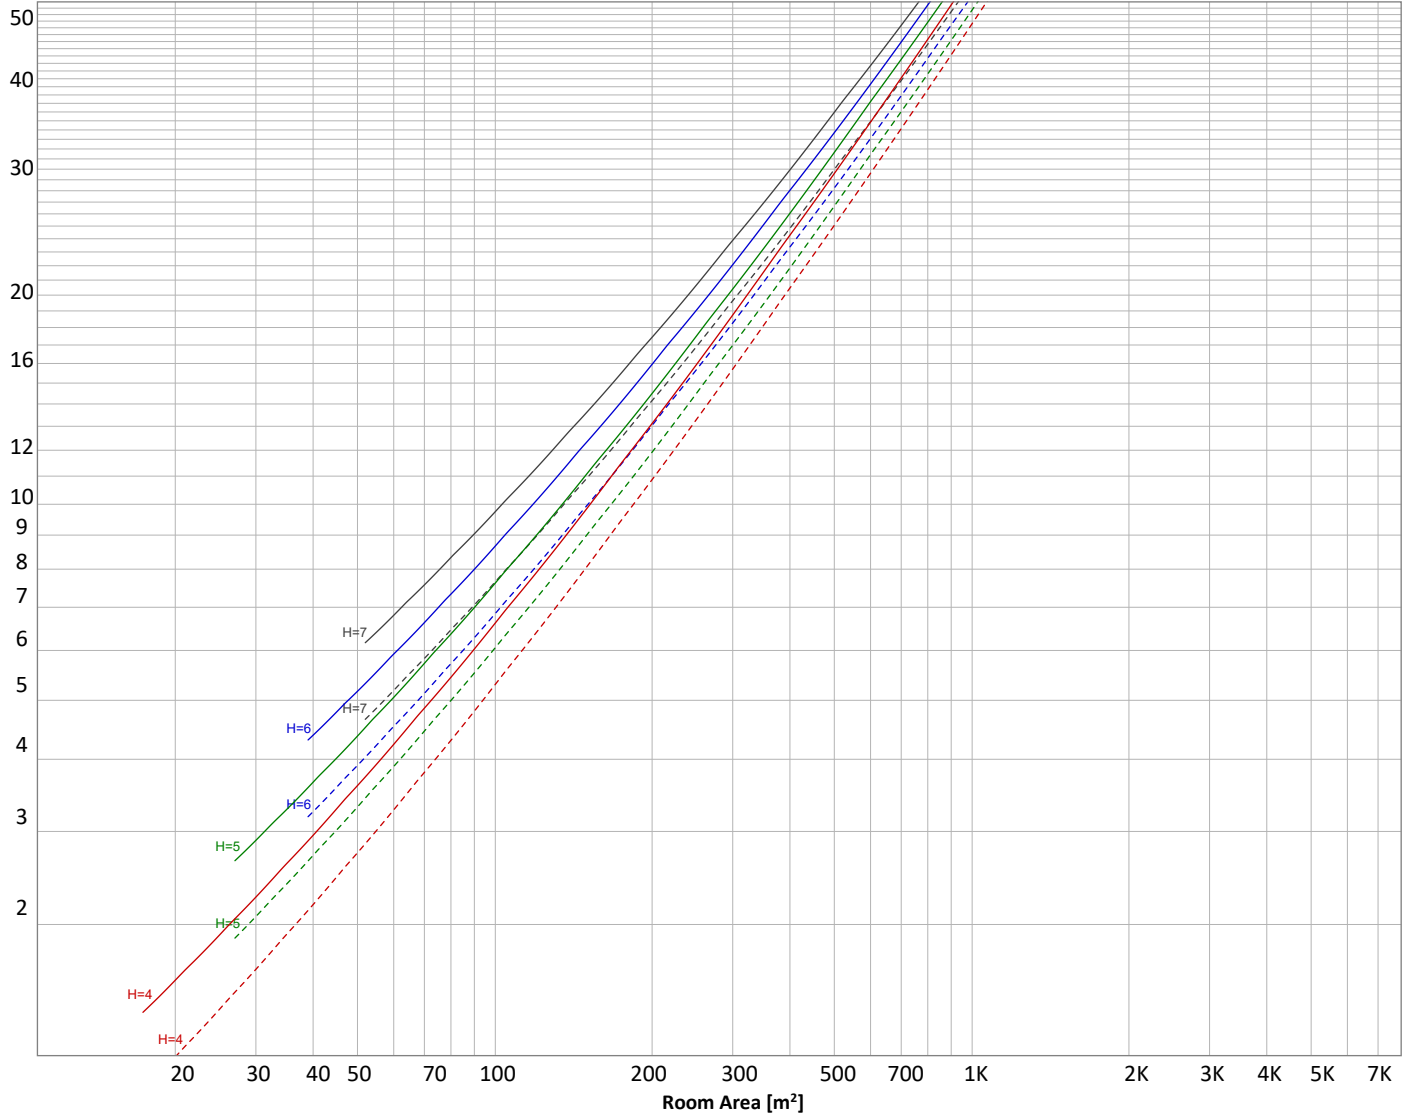

Conditions

H = Room height	Flux = 2245 lm				
H _{down} = Lamp distance from ceiling =	0.00 m	Line type	Ceiling reflectance	ρ(%) Wall reflectance	Floor reflectance
H _{work} = Work area height from floor =	0.00 m	-----	70	50	30
E _{work} = Average lux on work area =	100 lx	_____	50	30	20

Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
84,2 lm	246 lm	368 lm	399 lm	381 lm	302 lm	203 lm	116 lm	56,2 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
24,9 lm	20,1 lm	16,1 lm	11,9 lm	8,21 lm	4,53 lm	2,09 lm	0,831 lm	0,218 lm

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](#)

Operator:



Outdoor Light Planning

Lumen per Zone

Zone (γ)	Lumen	% Total
0-10°	84 lm	3,8%
10-20°	246 lm	11,0%
20-30°	368 lm	16,4%
30-40°	399 lm	17,8%
40-50°	381 lm	17,0%
50-60°	302 lm	13,4%
60-70°	203 lm	9,0%
70-80°	116 lm	5,2%
80-90°	56 lm	2,5%
90-100°	25 lm	1,1%
100-110°	20 lm	0,9%
110-120°	16 lm	0,7%
120-130°	12 lm	0,5%
130-140°	8 lm	0,4%
140-150°	5 lm	0,2%
150-160°	2 lm	0,1%
160-170°	1 lm	0,0%
170-180°	0 lm	0,0%
Total	2245 lm	100,0%

Intensity peaks

Max intensity	896 cd
Intensity, 90°	16 cd
Intensity, 0°	885 cd

Zonal Lumen summary


Zone (γ)	Lumen	% Total
0-30°	699 lm	31,1%
0-40°	1098 lm	48,9%
0-60°	1781 lm	79,3%
60-90°	375 lm	16,7%
70-100°	197 lm	8,8%
90-120°	61 lm	2,7%
0-90°	2156 lm	96,0%
90-180°	89 lm	4,0%
0-180°	2245 lm	100,0%

BUG rating

	Lumen	% Total
Forward light		
Low(0-30°)	348 lm	15,5%
Medium(30-60°)	541 lm	24,1%
High(60-80°)	160 lm	7,1%
Very high(80-90°)	28 lm	1,3%
Back light		
Low(0-30°)	348 lm	15,5%
Medium(30-60°)	541 lm	24,1%
High(60-80°)	160 lm	7,1%
Very high(80-90°)	28 lm	1,3%
Uplight		
Low(90-100°)	25 lm	1,1%
High(100-180°)	64 lm	2,8%

IESNA TM-15-07 Luminaire Classification System For Outdoor Luminaires

BUG rating B1 U3 G1

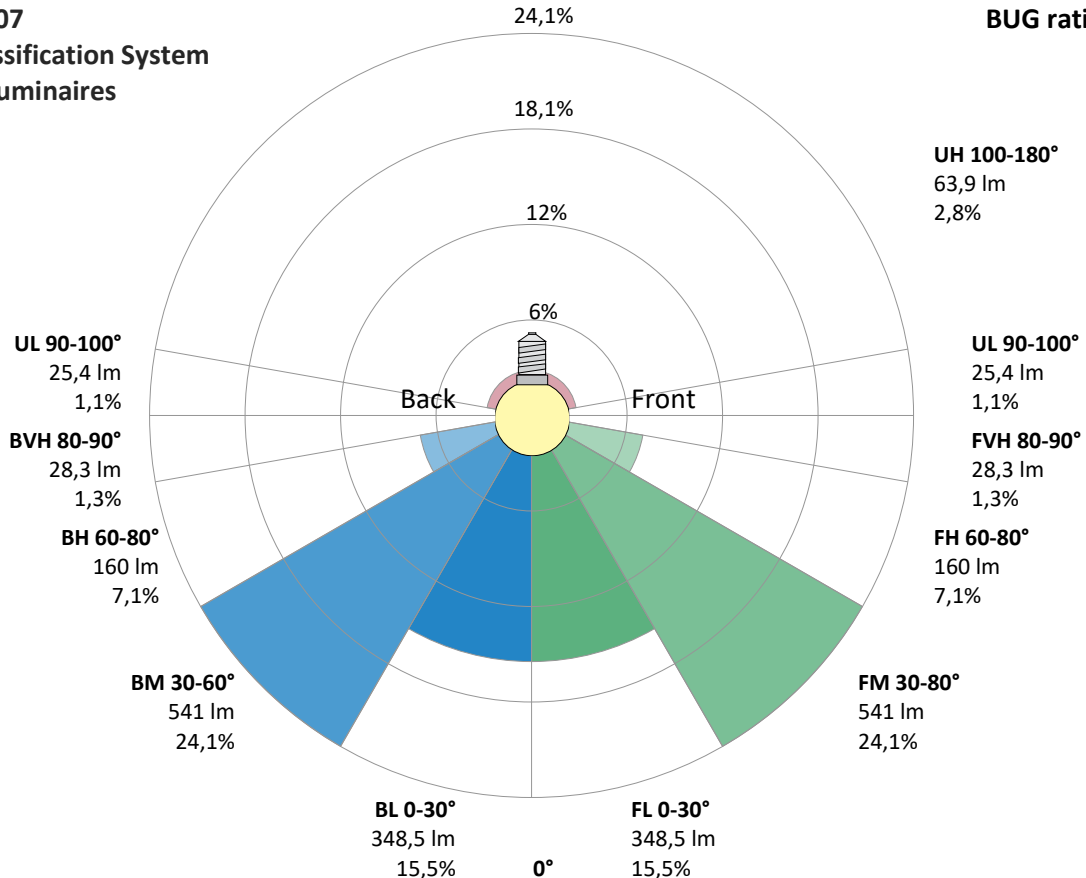

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](#)

Operator:




Power Details

Input Power

Power feed to light source	16,1 W
Frequency of input power	50 Hz
RMS Input voltage feed, V_{RMS}	230 V
RMS Input current feed, I_{RMS}	0,073 A
Volt-Ampere or apparent power = $V_{RMS} * I_{RMS}$	16,75 VA
Displacement factor of AC power feed	0,97
Power factor of AC current feed	0,96
Total harmonic distortion of the current	13,48%
Total harmonic distortion of the voltage	0,07%

Input Power Curve

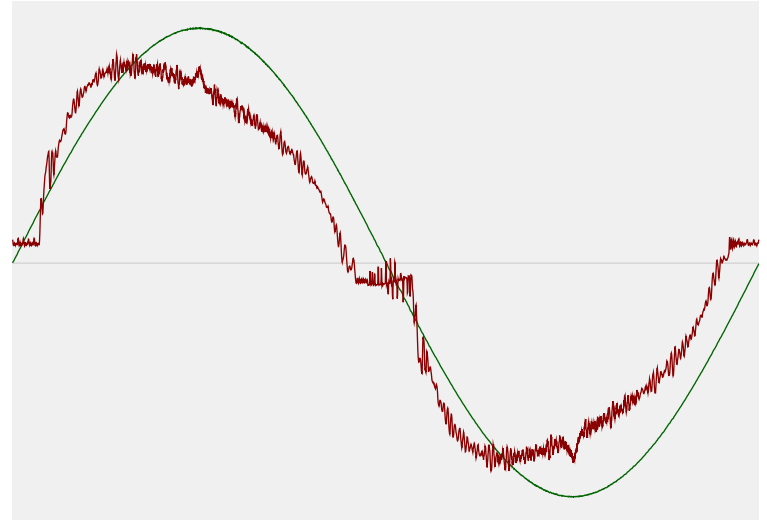

Efficiency

Radiated power efficiency	39,8%
Lumen efficiency	139 lm/W

Stabilization Details

Warmup Conditions

Stable period	15 min
Stable change max	2,0%
Minimum time	15 min

Color Temperature Change

CCT start	3000 K
CCT shift	+0 K
CCT end	3000 K


Warmup Result

Total warmup time	Lamp stabilized in 15 min 1 sec
Warmup variation	+0,1%

Output Change

Output start	2244 lm
Output change	+ lm
Output end	2245 lm

Stabilization Curve

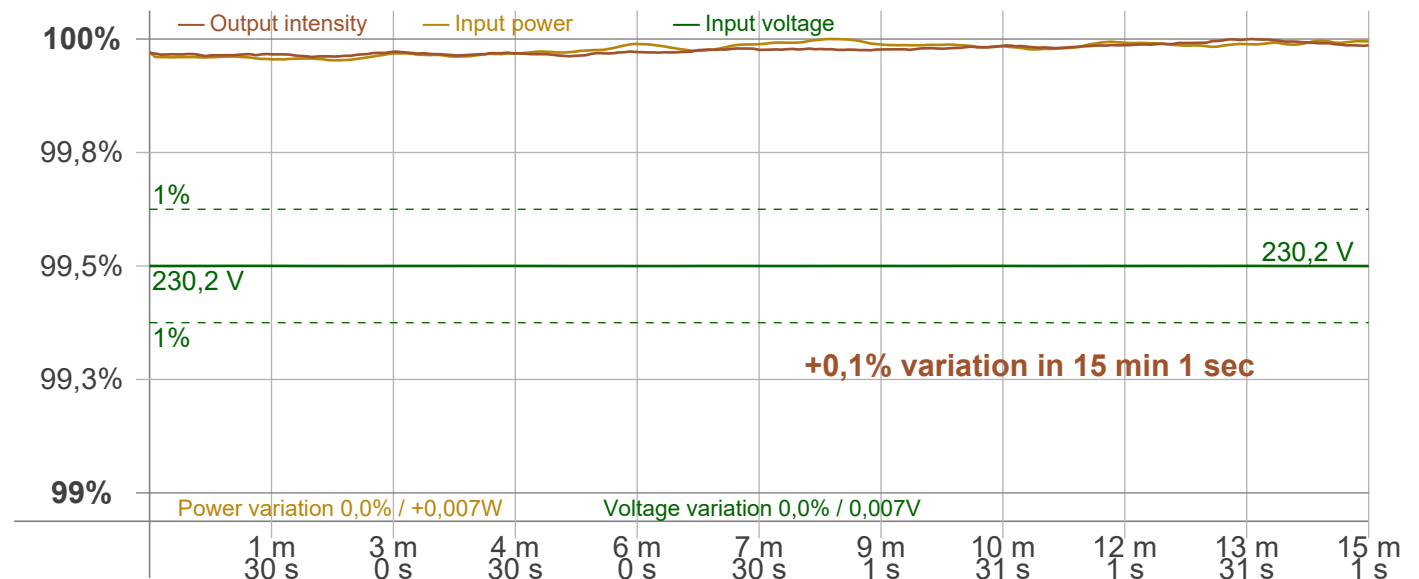

Light Measurement Report

Print date: 14-5-2025

Measurement date and time: 14-5-2025 09:34:15 – Measurement no. VFR-250514-1247-MS

Measurement tracking No. and Link: [VT250514-005869](#)

Operator:



Flicker /TLA details

Flicker Meter Type Viso Systems LabFlicker
 Frequency of input power 50 Hz
 Flicker/TLA sample rate 20000 samples/s

Measurement time
 PstLM 180 sec
 All other indices 1,2 sec

Flicker indices according to Illuminating Engineering Society (IES)

Flicker frequency 100 Hz
 Percent Flicker 0,87 %
 Flicker index 0

Flicker indices according to California Energy Commission (CEC) 2016b

JA8/10 40 Hz 0,07 %
 JA8/10 90 Hz 0,08 %
 JA8/10 200 Hz 0,85 %
 JA8/10 400 Hz 0,85 %
 JA8/10 1000 Hz 0,85 %


TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)

PstLM value (F < 80 Hz) 0,1
 SVM value (80 < F < 2000 Hz) 0,03

Flicker indices according to Lighting Research Center (2015)

Perception metric, Assist Mp 0,07

Flicker frame (frame of one flicker period in time domain)

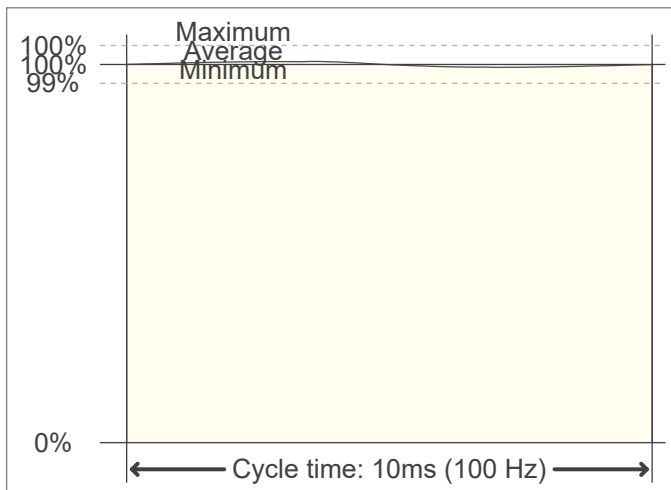

Flicker FFT (flicker curve in frequency domain)



IEEE 1789 Frequency/modulation plot

