

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](#)

Operator:



## Laboratory and Equipment

Laboratory Owner and Location  
Goniospectrometer System and Type  
Sensor Name, Calibr. Date and Serial No.  
Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark  
LabSpion – Type C, horizontal  
LabSensor Model2 – 11-1-2024 – 3130191315  
Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

## Measurement Conditions

Number of C-planes and Resolution  
 $\gamma$  (gamma)-Resolution  
Test Distance  
Input Power, Power and Displ. Factors  
Input RMS Voltage and Current  
Frequency of Input Power  
Warm-up Time and Variation

12 planes – 30°  
5°  
1,99 m  
9,9 W – PF 0,92 – DPF 0,97  
230 V – 0,047 A  
50 Hz  
Lamp stabilized in 23 min 49 sec – 2,0%

## Tested Light Source



Product Name  
Item No. and Manufacturer  
Product Description (line 1)

DR-MW090-4000K  
DR-MW090-4000K – Dutchfulfillment  
LED INBOUWSPOT MIRACLE 9W DIM WIT

## Main Light Measurement Results

Output – Total Lumen (Up% / Down%)  
Efficiency  
Peak Intensity and Beam Angle  
Correlated Color Temperature, Target/Measured  
Color Rendering Index  
Color Rendering TM30-18  
Color Shift, CIE duv and MacAdam Steps  
Flicker

840 lm – 0,05% / 99,95%  
85 lm/W  
863 cd – 62,7°  
CCT = 4000 K / 4049 K  
CRI 83,2  
 $R_f$  84,3 –  $R_g$  95,8  
Duv 0,0004 – SDCM 1,1  
SVM 1,09 – PstLM 0,03

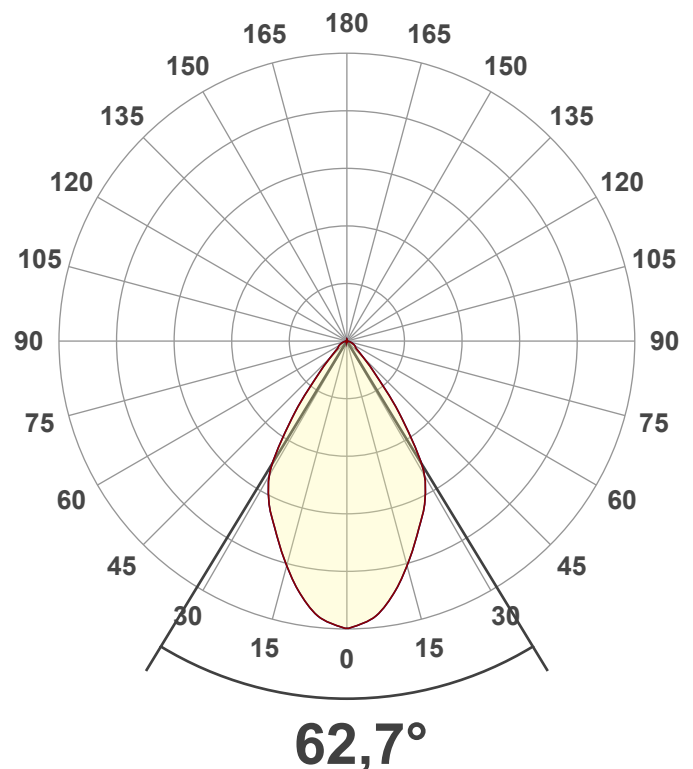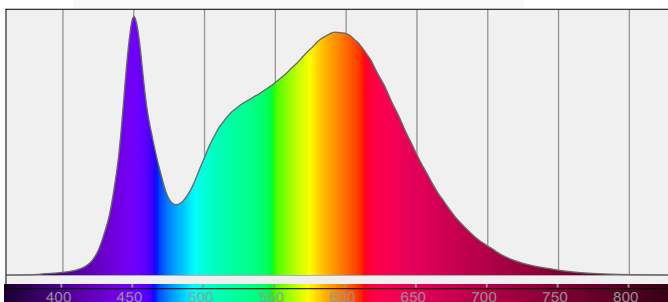

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS


Measurement tracking No. and Link: [VT250623-004415](#)

Operator:



## Luminous Intensity diagram

Unit: 0-100% of peak intensity

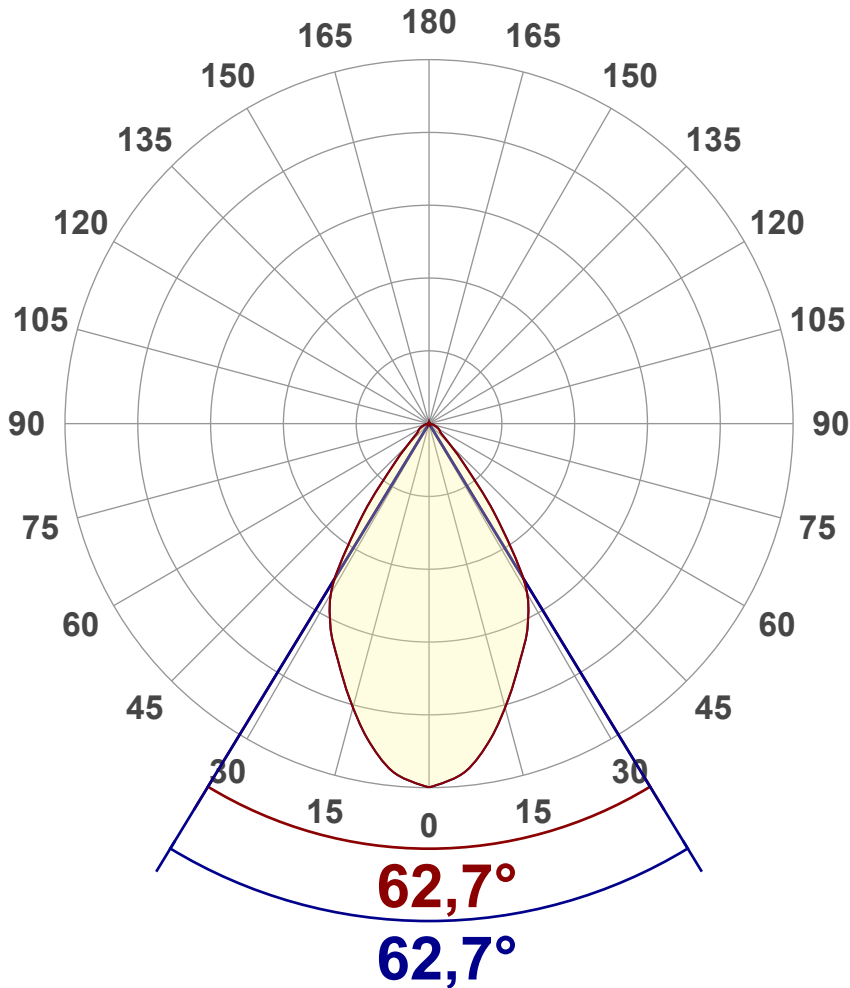

### Main Values

Output (total Lumen)	840 lm
Lumen Up% / Down%	0,05% / 99,95%
Peak Intensity	863 cd
Beam Angle (50%)	62,7°
Beam Angle (90%)	62,7°
Beam Angle (10%)	62,7°

### Cut-off Angle

Average 2,5%	129,7°
--------------	--------

### Field Angle

Average 10%	88,3°
-------------	-------


### Intensity Ratio

In 120° cone	95,8%
In 90° cone	89,7%

**C000-C180**

**C090-C270**

## Linear distribution diagram - Intensity (candela) vs $\gamma$ -angle

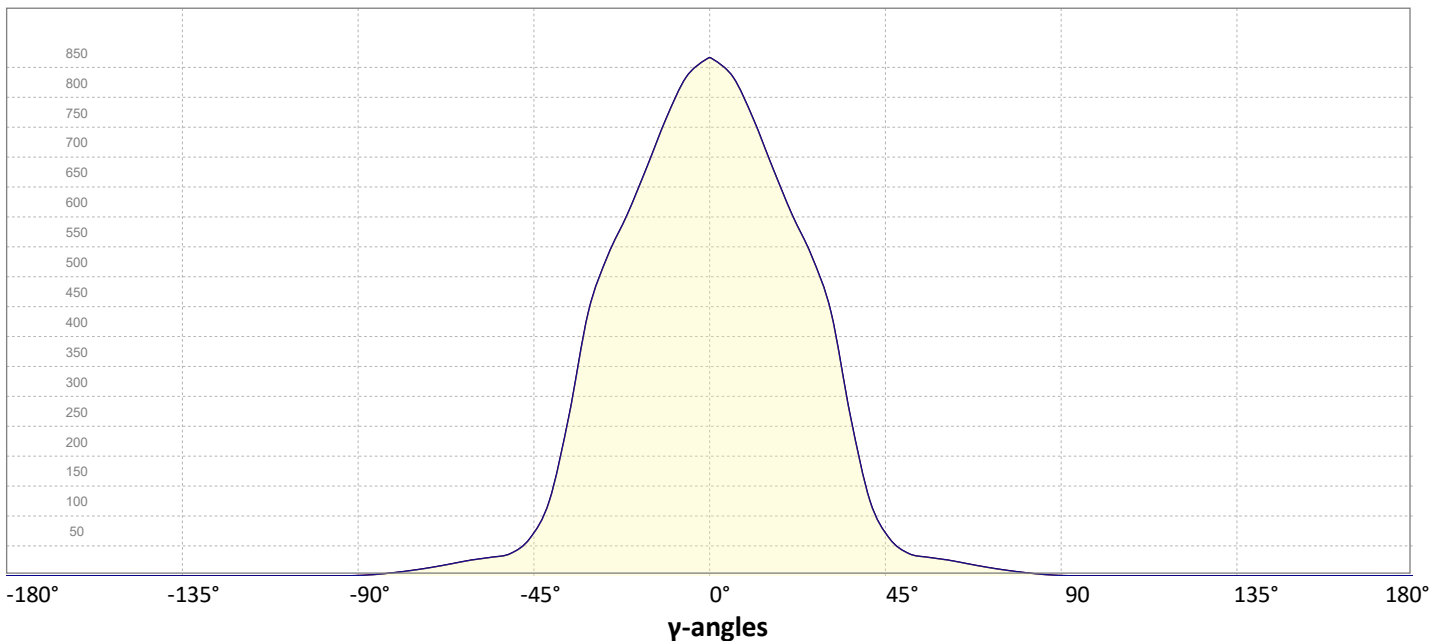

# Light Measurement Report

Print date: 23-6-2025


Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](#)

Operator:



## Iso-intensity Diagram (Iso-candela)

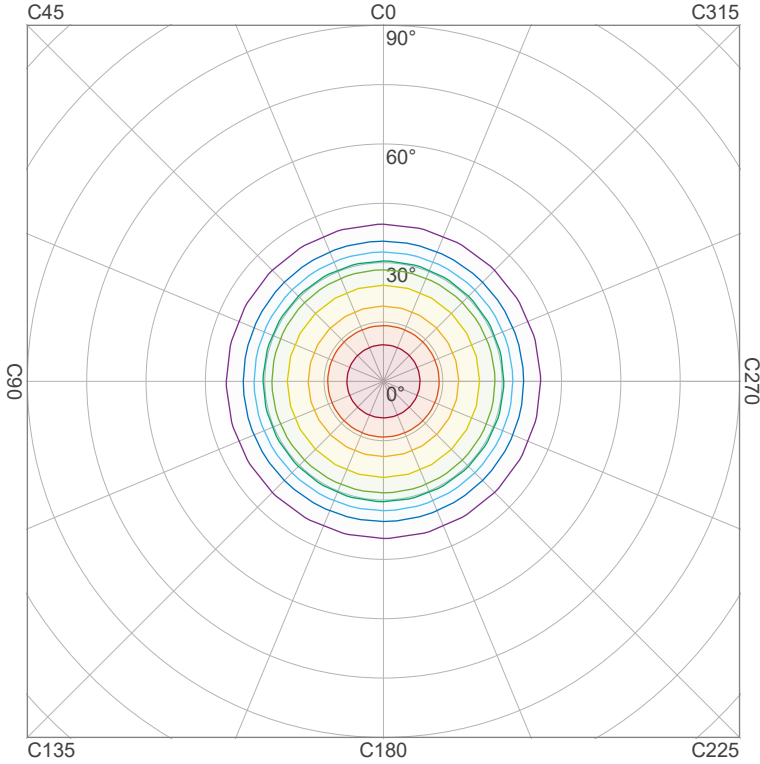


90 %	776,4 cd
80 %	690,2 cd
70 %	603,9 cd
60 %	517,6 cd
50 %	431,3 cd
40 %	345,1 cd
30 %	258,8 cd
20 %	172,5 cd
10 %	86,3 cd

Peak intensity: 862,7 cd

Number of c-planes: 12

## Iso-illuminance Diagram (Iso-lux)

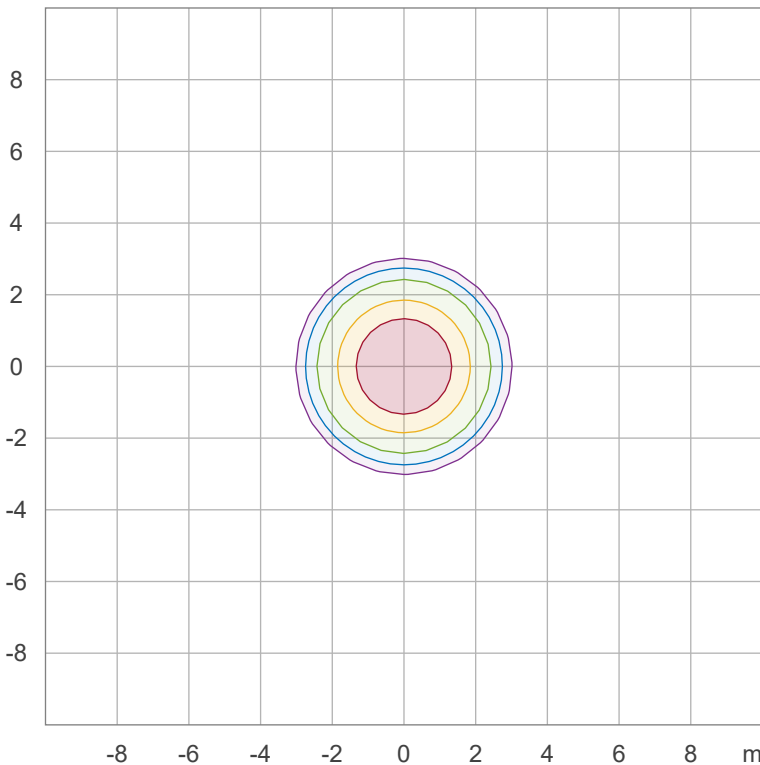

50,0 %	47,9 lx
30,0 %	28,8 lx
10,0 %	9,6 lx
5,0 %	4,8 lx
3,0 %	2,9 lx

Peak illuminance: 95,9 lx

Mounting height: 3,0 m

Number of c-planes: 12

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](https://www.viso-systems.com/VT250623-004415)

Operator:




## Color details


Correlated Color Temperature, Target CCT = 4000 K  
 Correlated Color Temperature, Measured CCT = 4049 K  
 Color Rendering Index CRI 83,2  
 Color Rendering Index, R9 (red component) R9 = 7,4  
 Color Rendering TM30-18 R<sub>f</sub> 84,3 – R<sub>g</sub> 95,8  
 Color Quality Scale CQS = 82,4

MacAdam Steps  
 Color coordinates CIE 1931 (x;y) = (0,381;0,377)  
 Color coordinate CIEs 1960 (u;v) = (0,225;0,334)  
 Color deviation from BBL Duv = 0,0004  
 Color coordinate CIEs 1976 (CIELUV) (u';v') = (0,225;0,502)


### CIE 1931

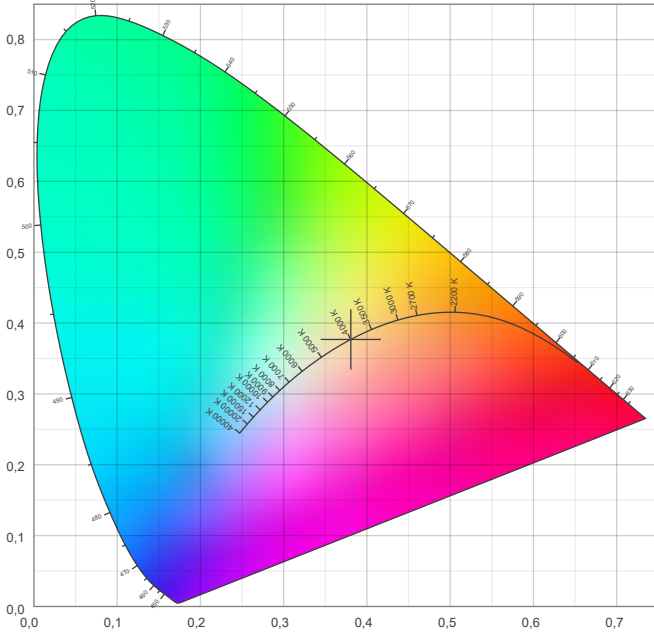

### CIE 1931 – zoomed on Planckian locus

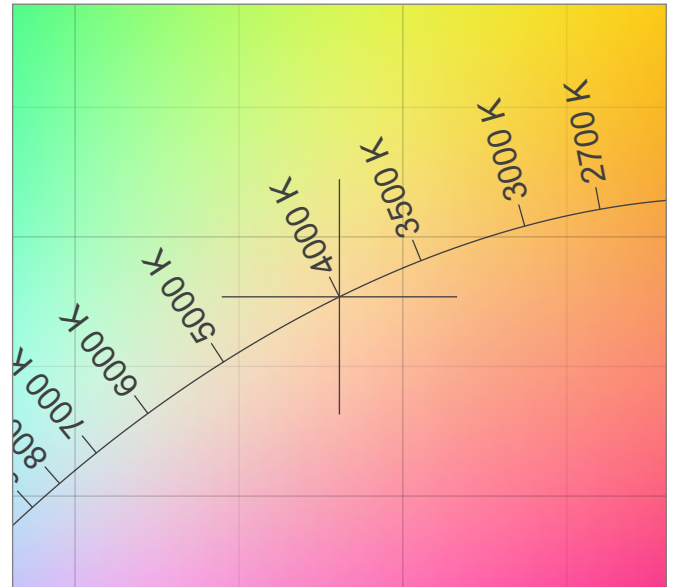


### Color Rendering Index per reference color (CIE 1995)

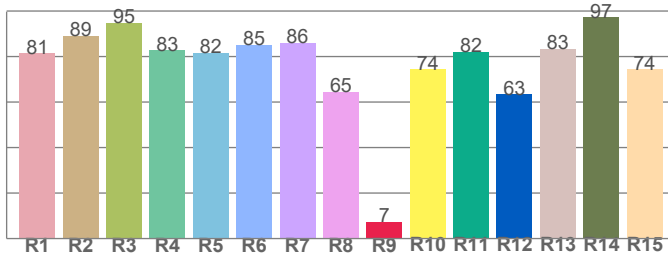


CRI R values, only R1-R8 are used to calculate final CRI value

R1	R2	R3	R4	R5	R6	R7	R8	R9	R10	R11	R12	R13	R14	R15
81,5	89,1	94,8	82,7	81,6	85,1	86,0	64,5	7,4	74,3	82,1	63,3	83,5	97,3	74,4

### Spectral power distribution (SPD) / W/nm – 0-100%

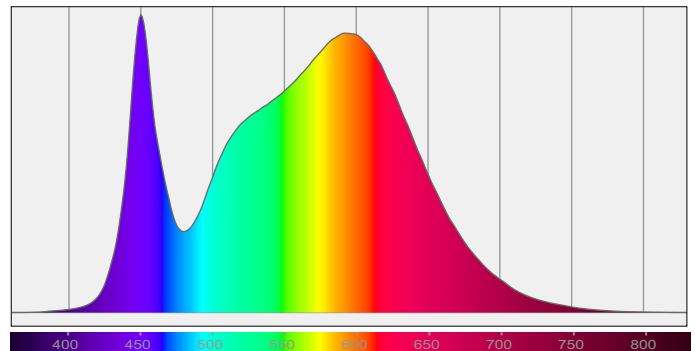


### TM30-18 Rf-values per hue bin

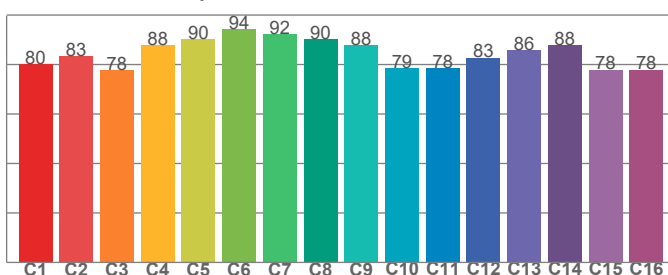

TM30 C values, 16 binned values out of total of 99 C values

C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
80,2	83,3	77,7	87,7	90,1	94,3	92,2	90,1	87,8	78,6	78,4	82,8	85,8	87,9	77,9	78,0

### Color Quality Scale by reference color

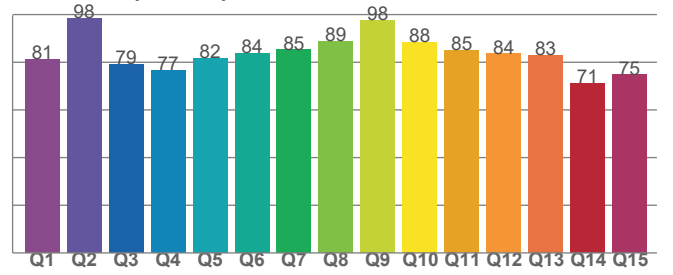

CQS Q values

Q1	Q2	Q3	Q4	Q5	Q6	Q7	Q8	Q9	Q10	Q11	Q12	Q13	Q14	Q15
81,2	98,5	79,3	76,6	81,8	83,7	85,3	88,8	97,7	88,3	85,1	83,5	83,0	71,2	74,8

# Light Measurement Report

Print date: 23-6-2025


Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](https://www.viso-systems.com/VT250623-004415)

Operator:



## Beam Details

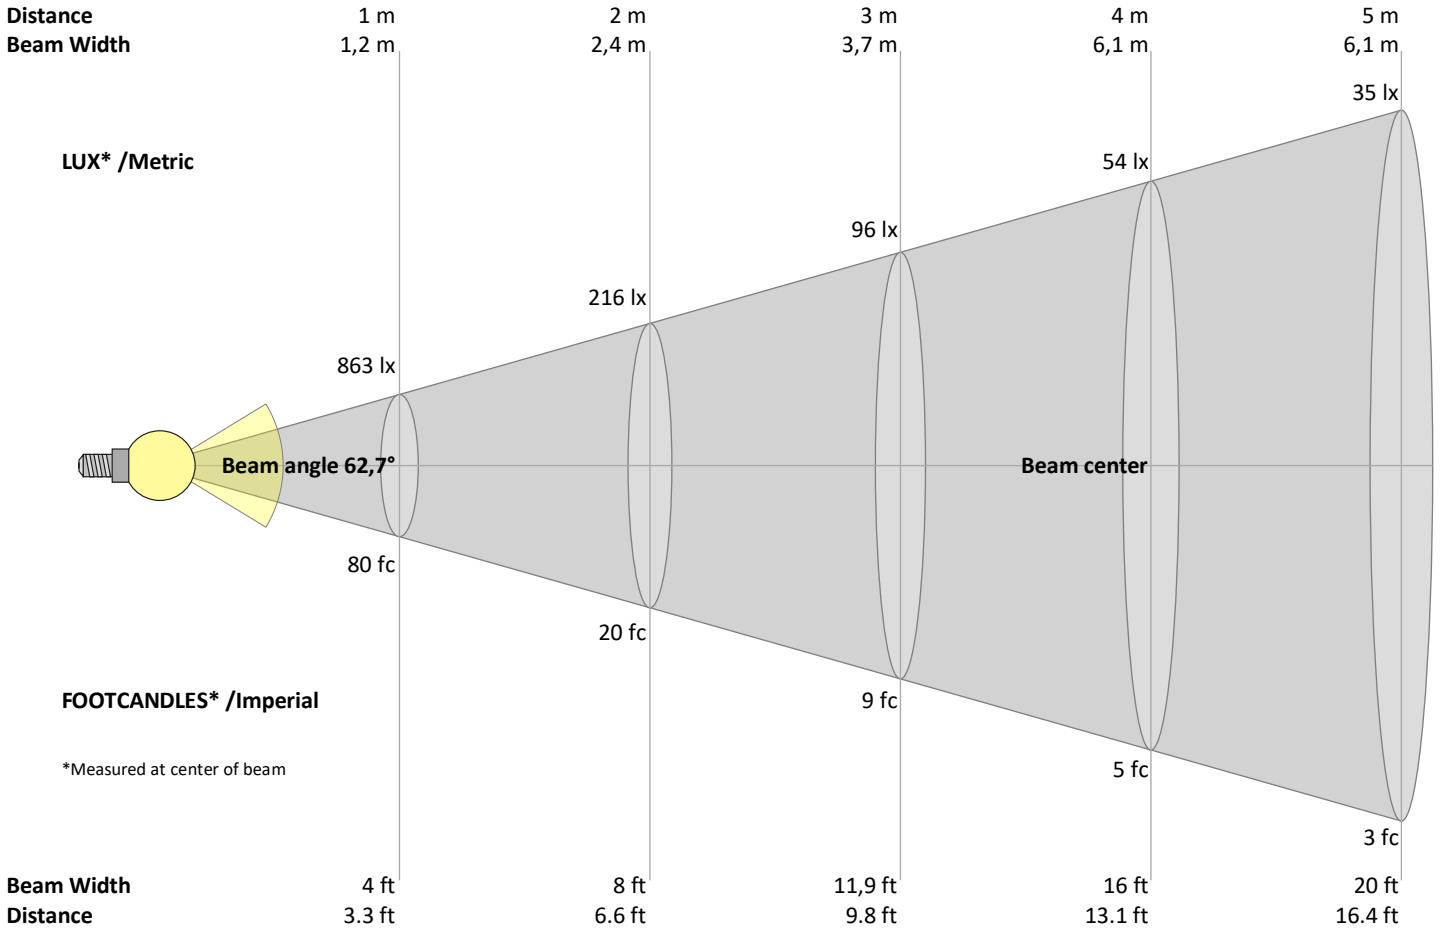

### Beam intensities from 1 – 20 m

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	m
3,3	6,6	9,8	13,1	16,4	19,7	23	26,2	29,5	32,8	36,1	39,4	42,7	45,9	49,2	52,5	55,8	59,1	62,3	65,6	ft
863	216	96	54	35	24	18	13	11	9	7	6	5	4	4	3	3	3	2	2	lux
80,1	20	8,9	5	3,2	2,2	1,6	1,3	1	0,8	0,7	0,6	0,5	0,4	0,4	0,3	0,3	0,2	0,2	0,2	fc

### Intensities in 0° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°	γ
863	857	845	834	807	780	750	717	684	653	621	592	564	536	499	461	408	338	268	211	cd
100%	99%	98%	97%	94%	90%	87%	83%	79%	76%	72%	69%	65%	62%	58%	53%	47%	39%	31%	24%	of 0°val

### Intensities in 90° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°	γ
863	857	845	834	807	780	750	717	684	653	621	592	564	536	499	461	408	338	268	211	cd
100%	99%	98%	97%	94%	90%	87%	83%	79%	76%	72%	69%	65%	62%	58%	53%	47%	39%	31%	24%	of 0°val

### Intensities in 180° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°	γ
863	857	845	834	807	780	750	717	684	653	621	592	564	536	499	461	408	338	268	211	cd
100%	99%	98%	97%	94%	90%	87%	83%	79%	76%	72%	69%	65%	62%	58%	53%	47%	39%	31%	24%	of 0°val

### Intensities in 270° c-plane

0°	2°	4°	6°	8°	10°	12°	14°	16°	18°	20°	22°	24°	26°	28°	30°	32°	34°	36°	38°	γ
863	857	845	834	807	780	750	717	684	653	621	592	564	536	499	461	408	338	268	211	cd
100%	99%	98%	97%	94%	90%	87%	83%	79%	76%	72%	69%	65%	62%	58%	53%	47%	39%	31%	24%	of 0°val

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](#)

Operator:



## Light Planning – UGR table

Uncorrected, comprehensive UGR table according to 117-1995

Reflectances		70	70	50	50	30	70	70	50	50	30
	ρ Ceiling	70	70	50	50	30	70	70	50	50	30
	ρ Walls	50	30	50	30	30	50	30	50	30	30
	ρ Floor	20	20	20	20	20	20	20	20	20	20
Room size		Viewed Crosswise					Viewed Endwise				
H = mounting height above eye level		(Viewing direction orthogonal to lamp length axis)					(Viewing direction parallel to lamp length axis)				
X	Y										
2H	2H	23,6	24,4	23,8	24,6	24,8	23,6	24,4	23,8	24,6	24,8
	3H	23,8	24,7	24,2	24,9	25,1	23,8	24,7	24,2	24,9	25,1
	4H	23,9	24,7	24,3	25,0	25,2	23,9	24,7	24,3	25,0	25,2
	6H	24,1	24,7	24,4	25,0	25,4	24,1	24,7	24,4	25,0	25,4
	8H	24,0	24,7	24,4	25,0	25,4	24,0	24,7	24,4	25,0	25,4
	12H	24,0	24,7	24,4	25,0	25,5	24,0	24,7	24,4	25,0	25,5
4H	2H	23,5	24,4	23,9	24,6	24,8	23,5	24,4	23,9	24,6	24,8
	3H	24,0	24,7	24,4	25,0	25,5	24,0	24,7	24,4	25,0	25,5
	4H	24,2	24,8	24,6	25,2	25,7	24,2	24,8	24,6	25,2	25,7
	6H	24,3	24,9	24,8	25,2	25,6	24,3	24,9	24,8	25,2	25,6
	8H	24,3	24,9	24,8	25,2	25,6	24,3	24,9	24,8	25,2	25,6
	12H	24,3	24,7	24,8	25,1	25,6	24,3	24,7	24,8	25,1	25,6
8H	4H	24,2	24,7	24,7	25,1	25,5	24,2	24,7	24,7	25,1	25,5
	6H	24,4	24,8	24,9	25,2	25,8	24,4	24,8	24,9	25,2	25,8
	8H	24,5	24,8	25,0	25,3	25,9	24,5	24,8	25,0	25,3	25,9
	12H	24,5	24,8	25,1	25,3	25,9	24,5	24,8	25,1	25,3	25,9
12H	4H	24,1	24,6	24,6	25,0	25,5	24,1	24,6	24,6	25,0	25,5
	6H	24,4	24,7	24,9	25,2	25,9	24,4	24,7	24,9	25,2	25,9
	8H	24,5	24,7	25,0	25,2	25,8	24,5	24,7	25,0	25,2	25,8

### Variations with the observer position for the luminaire spacings, S:

S = 1.0H	2,8 / -2,1	2,8 / -2,1
S = 1.5H	5,0 / -2,4	5,0 / -2,4
S = 2.0H	6,8 / -2,8	6,8 / -2,8

## Coefficients of Utilization

Ceiling reflectance	80			70			50			30			10			0		
Wall reflectance	70	50	30	10	70	50	30	10	50	30	10	50	30	10	50	30	10	0
Floor reflectance	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	0
RCR	(RCR: Room Cavity Ratio)																	
	Room Values are expressed as percentage of Lumen delivered to the task surface																	
0	119	119	119	119	116	116	116	116	111	111	106	106	106	102	102	102	100	100
1	113	110	107	104	110	107	105	103	103	101	99	99	98	96	96	95	94	92
2	106	101	96	92	104	99	95	91	96	92	89	93	90	87	90	88	86	84
3	100	93	88	83	98	92	87	82	89	85	81	86	83	80	84	81	79	77
4	95	86	80	75	93	85	79	75	83	78	74	81	77	73	79	75	72	71
5	89	80	74	69	88	79	73	69	77	72	68	76	71	67	74	70	67	65
6	84	75	68	64	83	74	68	63	72	67	63	71	66	62	70	65	62	60
7	80	70	63	59	79	69	63	59	68	62	58	67	62	58	65	61	58	56
8	76	66	59	55	75	65	59	55	64	58	54	63	58	54	62	57	54	52
9	72	62	55	51	71	61	55	51	60	55	51	59	54	51	58	54	50	49
10	68	58	52	48	67	58	52	48	57	51	48	56	51	47	55	51	47	46

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](https://www.viso-systems.com/VT250623-004415)


Operator:



## Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

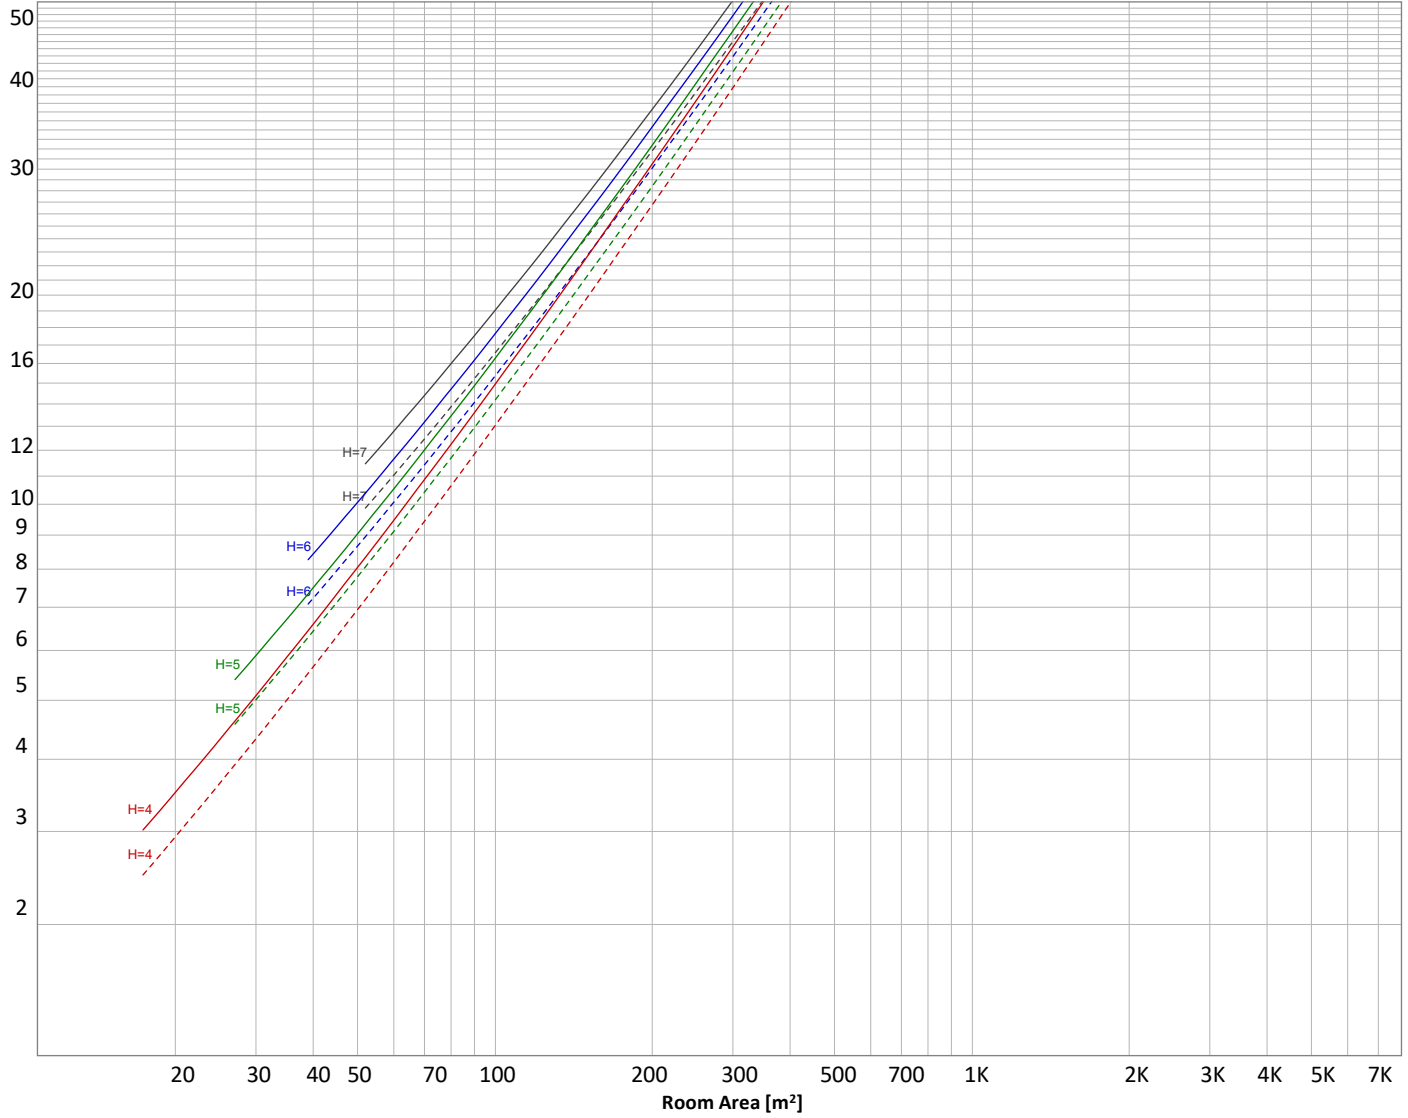

### Conditions

H = Room height	Flux = 840 lm				
H <sub>down</sub> = Lamp distance from ceiling =	0.00 m	Line type	Ceiling reflectance	ρ(%) Wall reflectance	Floor reflectance
H <sub>work</sub> = Work area height from floor =	0.00 m	-----	70	50	30
E <sub>work</sub> = Average lux on work area =	100 lx	_____	50	30	20

### Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
78,2 lm	196 lm	251 lm	189 lm	61,5 lm	28,9 lm	21,2 lm	10,9 lm	3,04 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
0,114 lm	0,016 lm	0,012 lm	0,020 lm	0,030 lm	0,073 lm	0,076 lm	0,054 lm	0,018 lm

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](https://www.viso-systems.com/VT250623-004415)

Operator:



## Outdoor Light Planning

### Lumen per Zone

Zone (γ)	Lumen	% Total
0-10°	78 lm	9,3%
10-20°	196 lm	23,4%
20-30°	251 lm	29,8%
30-40°	189 lm	22,5%
40-50°	61 lm	7,3%
50-60°	29 lm	3,4%
60-70°	21 lm	2,5%
70-80°	11 lm	1,3%
80-90°	3 lm	0,4%
90-100°	0 lm	0,0%
100-110°	0 lm	0,0%
110-120°	0 lm	0,0%
120-130°	0 lm	0,0%
130-140°	0 lm	0,0%
140-150°	0 lm	0,0%
150-160°	0 lm	0,0%
160-170°	0 lm	0,0%
170-180°	0 lm	0,0%
<b>Total</b>	<b>840 lm</b>	<b>100,0%</b>

### Intensity peaks

Max intensity	863 cd
Intensity, 90°	1 cd
Intensity, 0°	863 cd

### Zonal Lumen summary


Zone (γ)	Lumen	% Total
0-30°	525 lm	62,5%
0-40°	714 lm	85,0%
0-60°	804 lm	95,8%
60-90°	35 lm	4,2%
70-100°	14 lm	1,7%
90-120°	0 lm	0,0%
0-90°	839 lm	100,0%
90-180°	0 lm	0,0%
0-180°	840 lm	100,0%

### BUG rating

	Lumen	% Total
<b>Forward light</b>		
Low(0-30°)	262 lm	31,2%
Medium(30-60°)	140 lm	16,7%
High(60-80°)	16 lm	1,9%
Very high(80-90°)	2 lm	0,2%
<b>Back light</b>		
Low(0-30°)	262 lm	31,2%
Medium(30-60°)	140 lm	16,7%
High(60-80°)	16 lm	1,9%
Very high(80-90°)	2 lm	0,2%
<b>Uplight</b>		
Low(90-100°)	0 lm	0,0%
High(100-180°)	0 lm	0,0%

## IESNA TM-15-07 Luminaire Classification System For Outdoor Luminaires

BUG rating B1 U0 G0

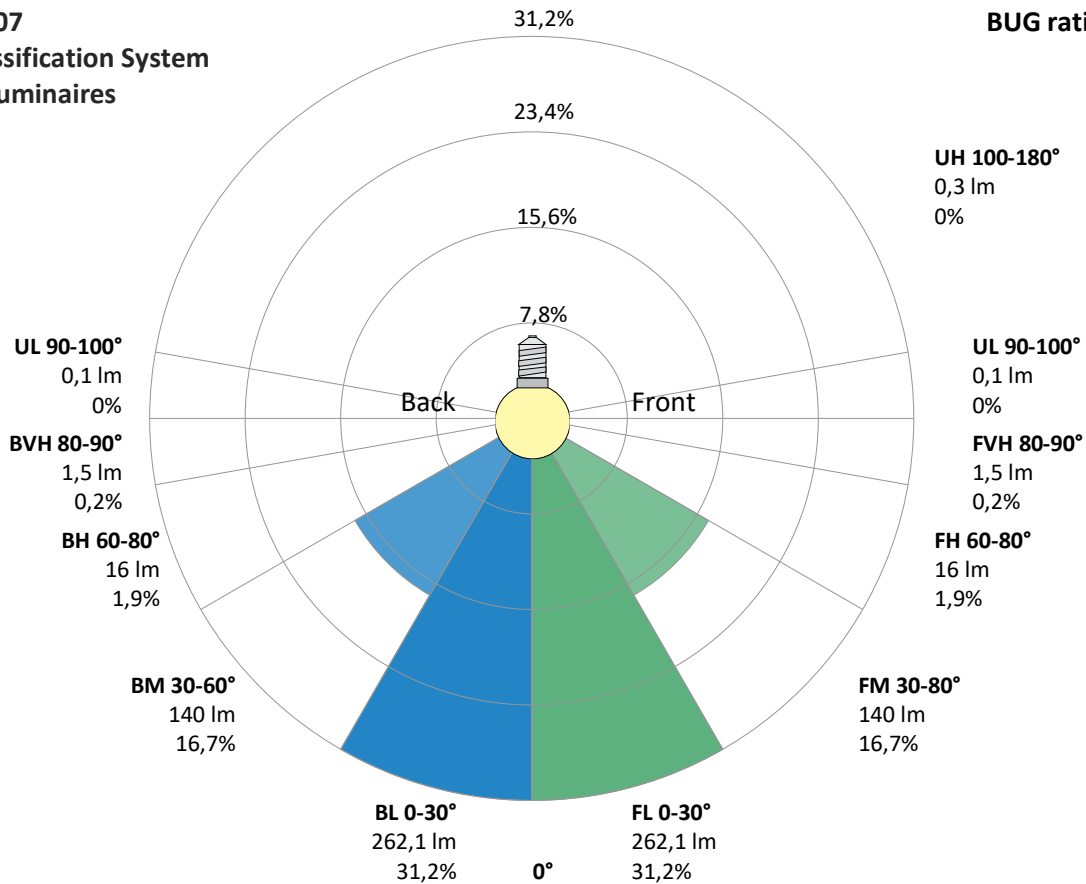

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](#)

Operator:




## Power Details


### Input Power

Power feed to light source	9,9 W
Frequency of input power	50 Hz
RMS Input voltage feed, $V_{RMS}$	230 V
RMS Input current feed, $I_{RMS}$	0,047 A
Volt-Ampere or apparent power = $V_{RMS} * I_{RMS}$	10,71 VA
Displacement factor of AC power feed	0,97
Power factor of AC current feed	0,92
Total harmonic distortion of the current	32,47%
Total harmonic distortion of the voltage	0,06%

### Input Power Curve

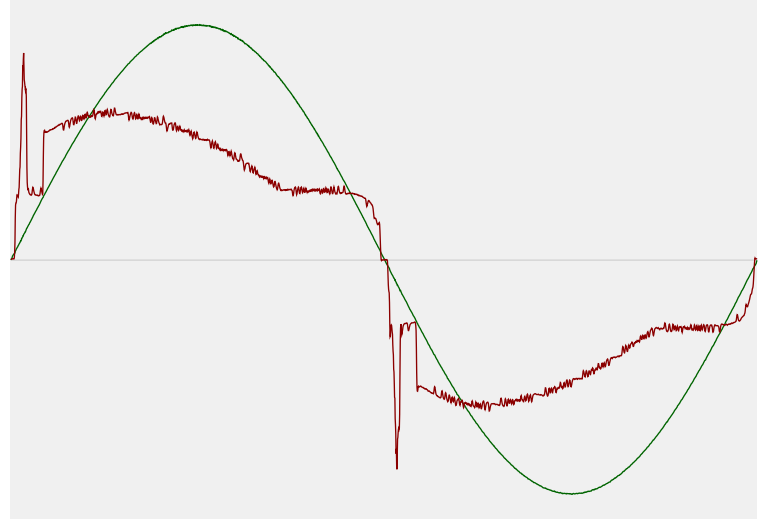

### Efficiency

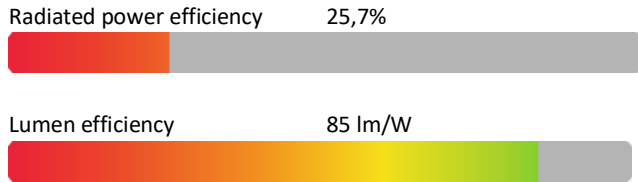

## Stabilization Details

### Warmup Conditions

Stable period	15 min
Stable change max	2,0%
Minimum time	15 min

### Color Temperature Change

CCT start	3970 K
CCT shift	+30 K
CCT end	4000 K


### Warmup Result

Total warmup time	Lamp stabilized in 23 min 49 sec
Warmup variation	-5,6%

### Output Change

Output start	889 lm
Output change	-49 lm
Output end	840 lm

## Stabilization Curve

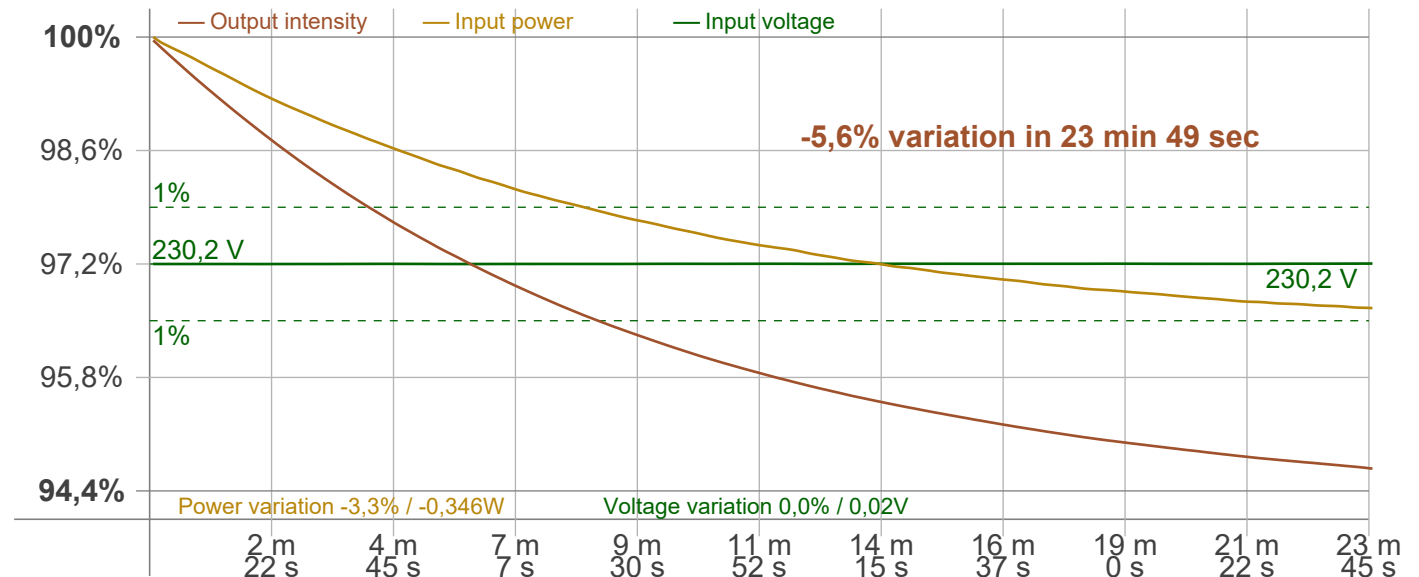

# Light Measurement Report

Print date: 23-6-2025

Measurement date and time: 23-6-2025 09:12:56 – Measurement no. VFR-250623-1686-MS

Measurement tracking No. and Link: [VT250623-004415](https://www.viso-systems.com/VT250623-004415)

Operator:



## Flicker /TLA details

Flicker Meter Type: Viso Systems LabFlicker  
 Frequency of input power: 50 Hz  
 Flicker/TLA sample rate: 20000 samples/s

**Measurement time**  
 PstLM: 180 sec  
 All other indices: 1,2 sec

### Flicker indices according to Illuminating Engineering Society (IES)

Flicker frequency: 100 Hz  
 Percent Flicker: 28,18 %  
 Flicker index: 0,09

### Flicker indices according to California Energy Commission (CEC) 2016b

JA8/10 40 Hz: 0,04 %  
 JA8/10 90 Hz: 0,24 %  
 JA8/10 200 Hz: 28,51 %  
 JA8/10 400 Hz: 28,31 %  
 JA8/10 1000 Hz: 28,17 %


### TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)

PstLM value (F < 80 Hz): 0,03  
 SVM value (80 < F < 2000 Hz): 1,09


### Flicker indices according to Lighting Research Center (2015)

Perception metric, Assist Mp: 0,01

Flicker frame (frame of one flicker period in time domain)

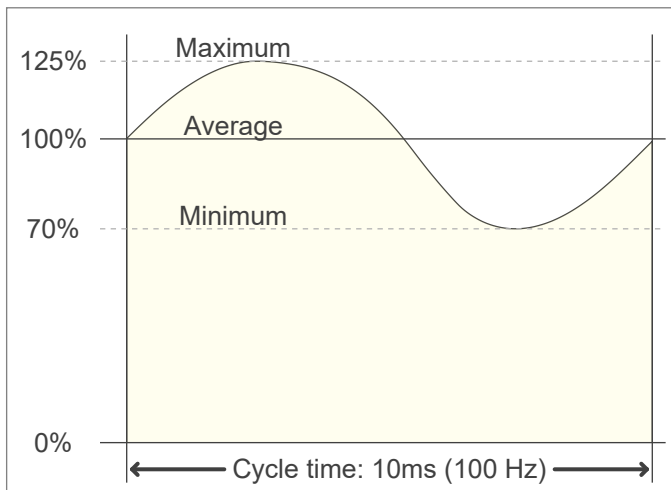

Flicker FFT (flicker curve in frequency domain)

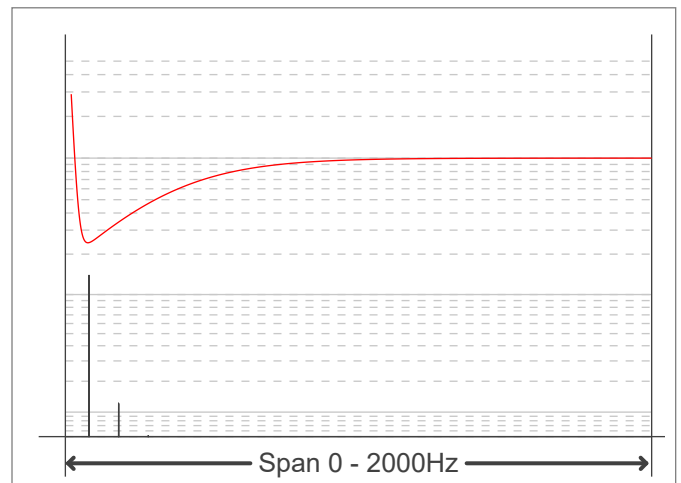

IEEE 1789 Frequency/modulation plot

