

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)

Operator:



Laboratory and Equipment

Laboratory Owner and Location
Goniospectrometer System and Type
Sensor Name, Calibr. Date and Serial No.
Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark
LabSpion – Type C, horizontal
LabSensor Model2 – 11-1-2024 – 3130191315
Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

Measurement Conditions

Number of C-planes and Resolution
 γ (gamma)-Resolution
Test Distance
Input Power, Power and Displ. Factors
Input RMS Voltage and Current
Frequency of Input Power
Warm-up Time and Variation

12 planes – 30°
5°
12,10 m
49,9 W – PF 0,98 – DPF 0,98
230 V – 0,222 A
50 Hz
Lamp stabilized in 15 min 1 sec – 2,0%

Tested Light Source



Product Name
Item No. and Manufacturer
Product Description (line 1)

812492-3000K
812492-3000K – Dutchfulfillment
LED BATTEN | CHARON | 150CM | 50W | CCT-SWITCH

Main Light Measurement Results

Output – Total Lumen (Up% / Down%)
Efficiency
Peak Intensity and Beam Angle
Correlated Color Temperature, Target/Measured
Color Rendering Index
Color Rendering TM30-18
Color Shift, CIE duv and MacAdam Steps
Flicker

5458 lm – 4,37% / 95,63%
109 lm/W
1709 cd – 114,2°
CCT = 3000 K / 6712 K
CRI 82,7
 R_f 83,0 – R_g 97,0
Duv 0,0059 – SDCM 59,0
SVM 0,01 – PstLM 0,01

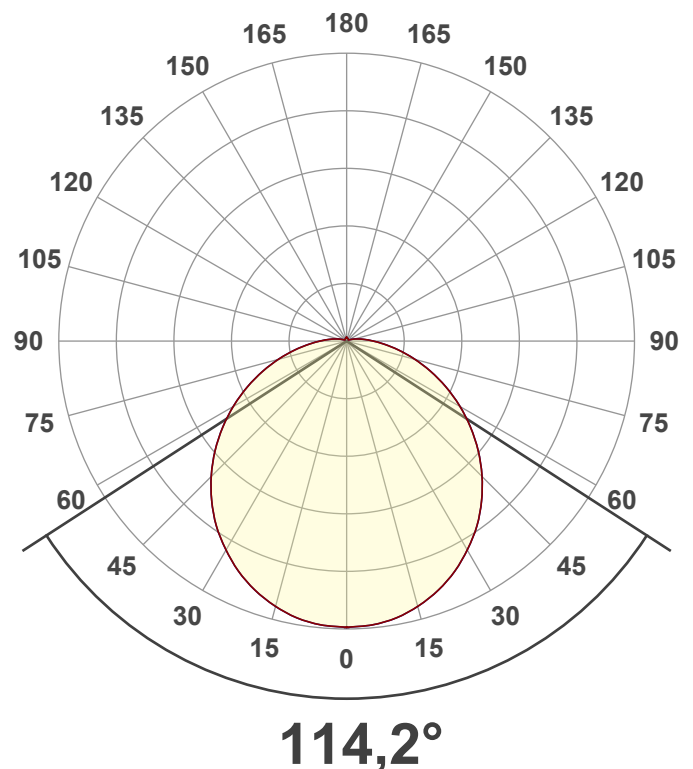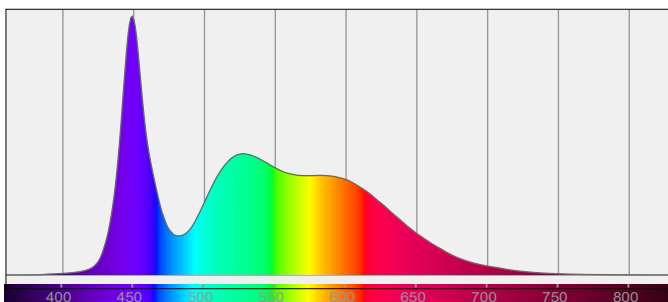

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS


Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)

Operator:



Luminous Intensity diagram

Unit: 0-100% of peak intensity

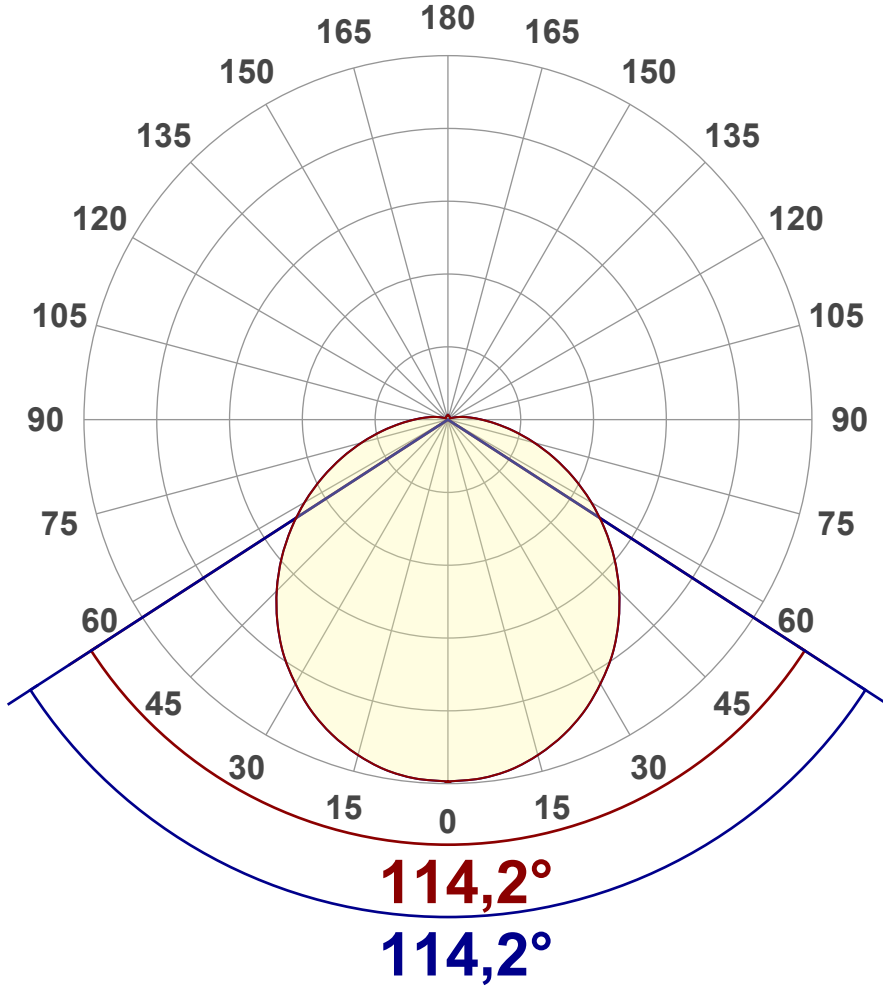

Main Values

Output (total Lumen)	5458 lm
Lumen Up% / Down%	4,37% / 95,63%
Peak Intensity	1709 cd
Beam Angle (50%)	114,2°
Beam Angle (90%)	114,2°
Beam Angle (10%)	114,2°

Cut-off Angle

Average 2,5%	211,4°
--------------	--------

Field Angle

Average 10%	178,4°
-------------	--------


Intensity Ratio

In 120° cone	70,8%
In 90° cone	47,9%

C000-C180

C090-C270

Linear distribution diagram - Intensity (candela) vs γ -angle

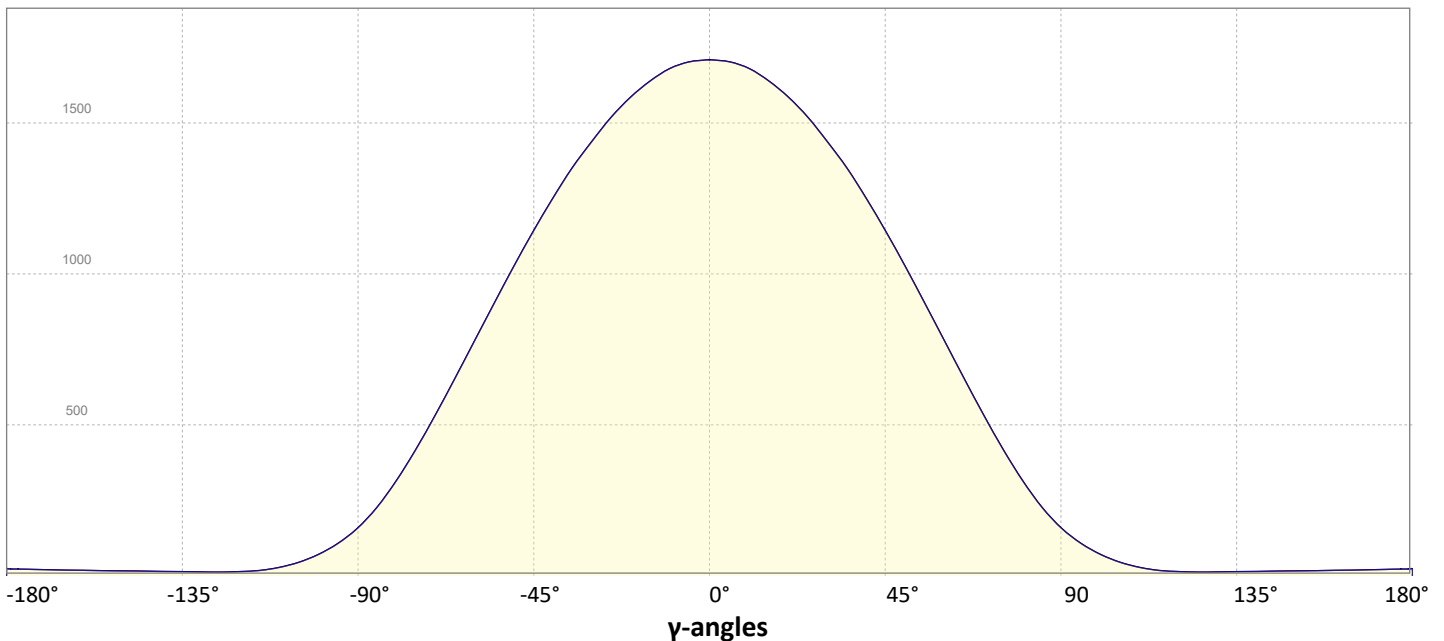

Light Measurement Report

Print date: 8-9-2025


Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://vt250908-000895)

Operator:



Iso-intensity Diagram (Iso-candela)

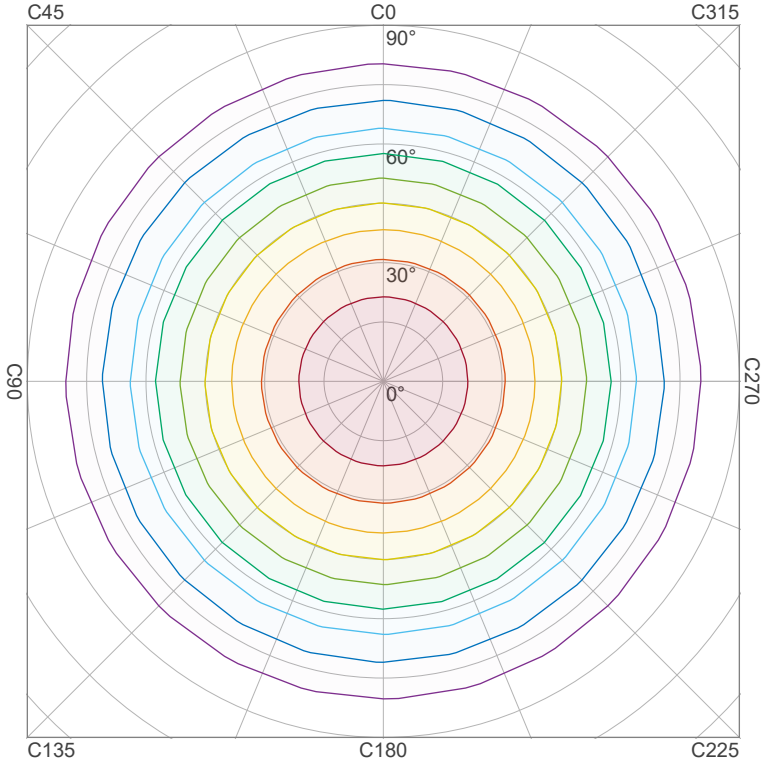


90 %	1538,4 cd
80 %	1367,5 cd
70 %	1196,5 cd
60 %	1025,6 cd
50 %	854,7 cd
40 %	683,7 cd
30 %	512,8 cd
20 %	341,9 cd
10 %	170,9 cd

Peak intensity: 1709,3 cd

Number of c-planes: 12

Iso-illuminance Diagram (Iso-lux)

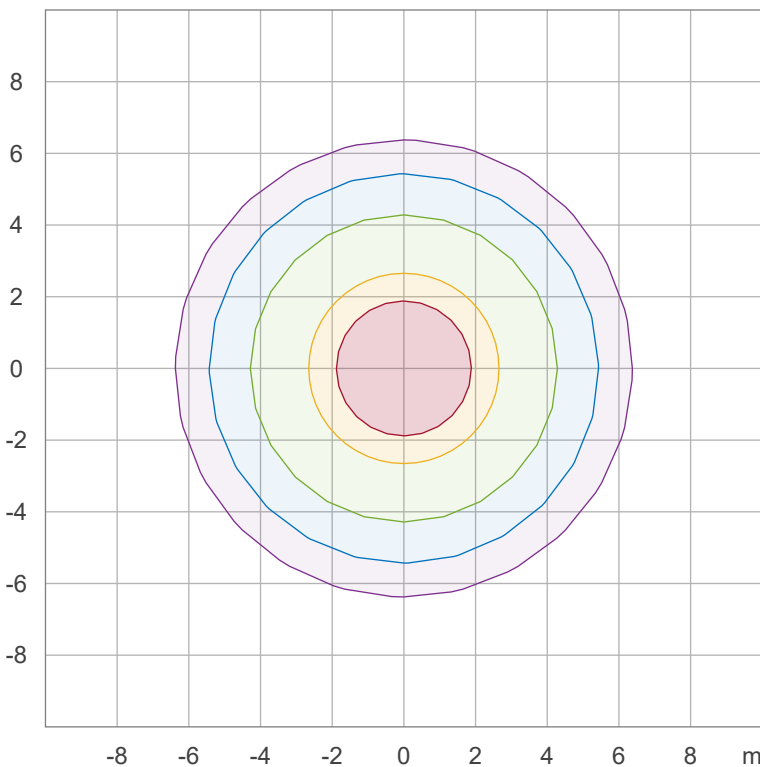

50,0 %	95,0 lx
30,0 %	57,0 lx
10,0 %	19,0 lx
5,0 %	9,5 lx
3,0 %	5,7 lx

Peak illuminance: 189,9 lx

Mounting height: 3,0 m

Number of c-planes: 12

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)

Operator:



Color details

Correlated Color Temperature, Target CCT = 3000 K
 Correlated Color Temperature, Measured CCT = 6712 K
 Color Rendering Index CRI 82,7
 Color Rendering Index, R9 (red component) R9 = 11,8
 Color Rendering TM30-18 R_f 83,0 – R_g 97,0
 Color Quality Scale CQS = 82,3

MacAdam Steps SDCM = 59,0
 Color coordinates CIE 1931 (x;y) = (0,437;0,404)
 Color coordinate CIEs 1960 (u;v) = (0,251;0,348)
 Color deviation from BBL Duv = 0,0059
 Color coordinate CIEs 1976 (CIELUV) (u';v') = (0,251;0,521)


CIE 1931



CIE 1931 – zoomed on Planckian locus




Color Rendering Index per reference color (CIE 1995)

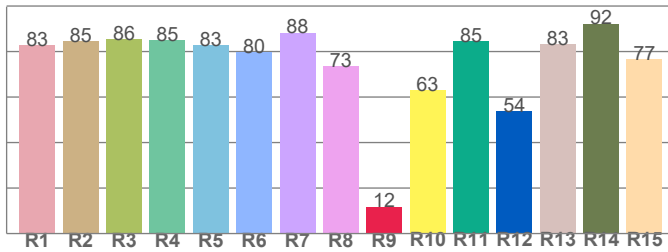


CRI R values, only R1-R8 are used to calculate final CRI value

R1	R2	R3	R4	R5	R6	R7	R8	R9	R10	R11	R12	R13	R14	R15
82,7	84,6	85,5	84,9	82,8	79,7	88,2	73,4	11,8	63,1	84,5	53,8	83,2	92,2	76,5

Spectral power distribution (SPD) / W/nm – 0-100%

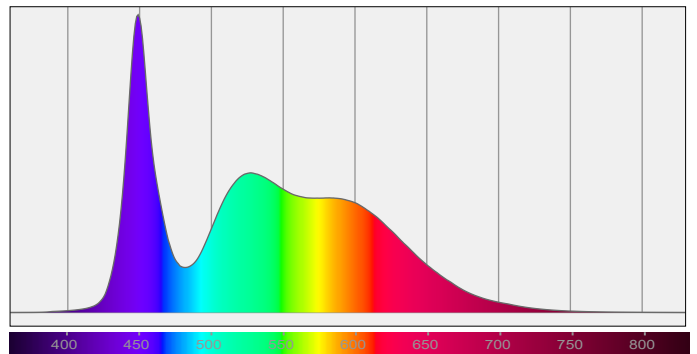


TM30-18 R_f-values per hue bin

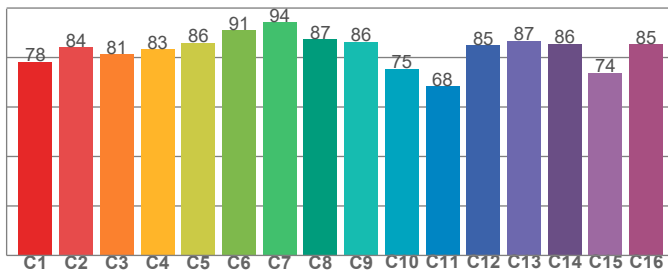

TM30 C values, 16 binned values out of total of 99 C values

C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
78,2	84,2	81,4	83,5	86,0	91,0	94,2	87,4	86,4	75,4	68,4	84,9	86,7	85,5	73,9	85,4

Color Quality Scale by reference color

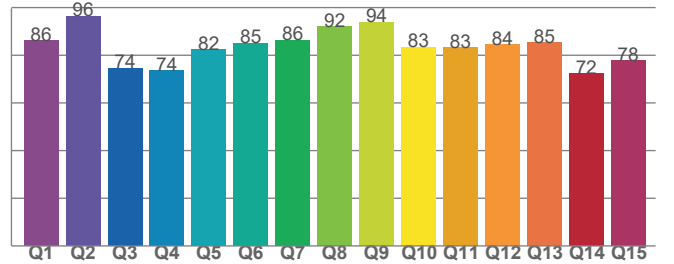

CQS Q values

Q1	Q2	Q3	Q4	Q5	Q6	Q7	Q8	Q9	Q10	Q11	Q12	Q13	Q14	Q15
86,1	96,3	74,5	73,5	82,2	85,0	86,3	91,9	93,8	83,4	83,1	84,3	85,3	72,3	77,8

Light Measurement Report

Print date: 8-9-2025


Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)

Operator:



Beam Details

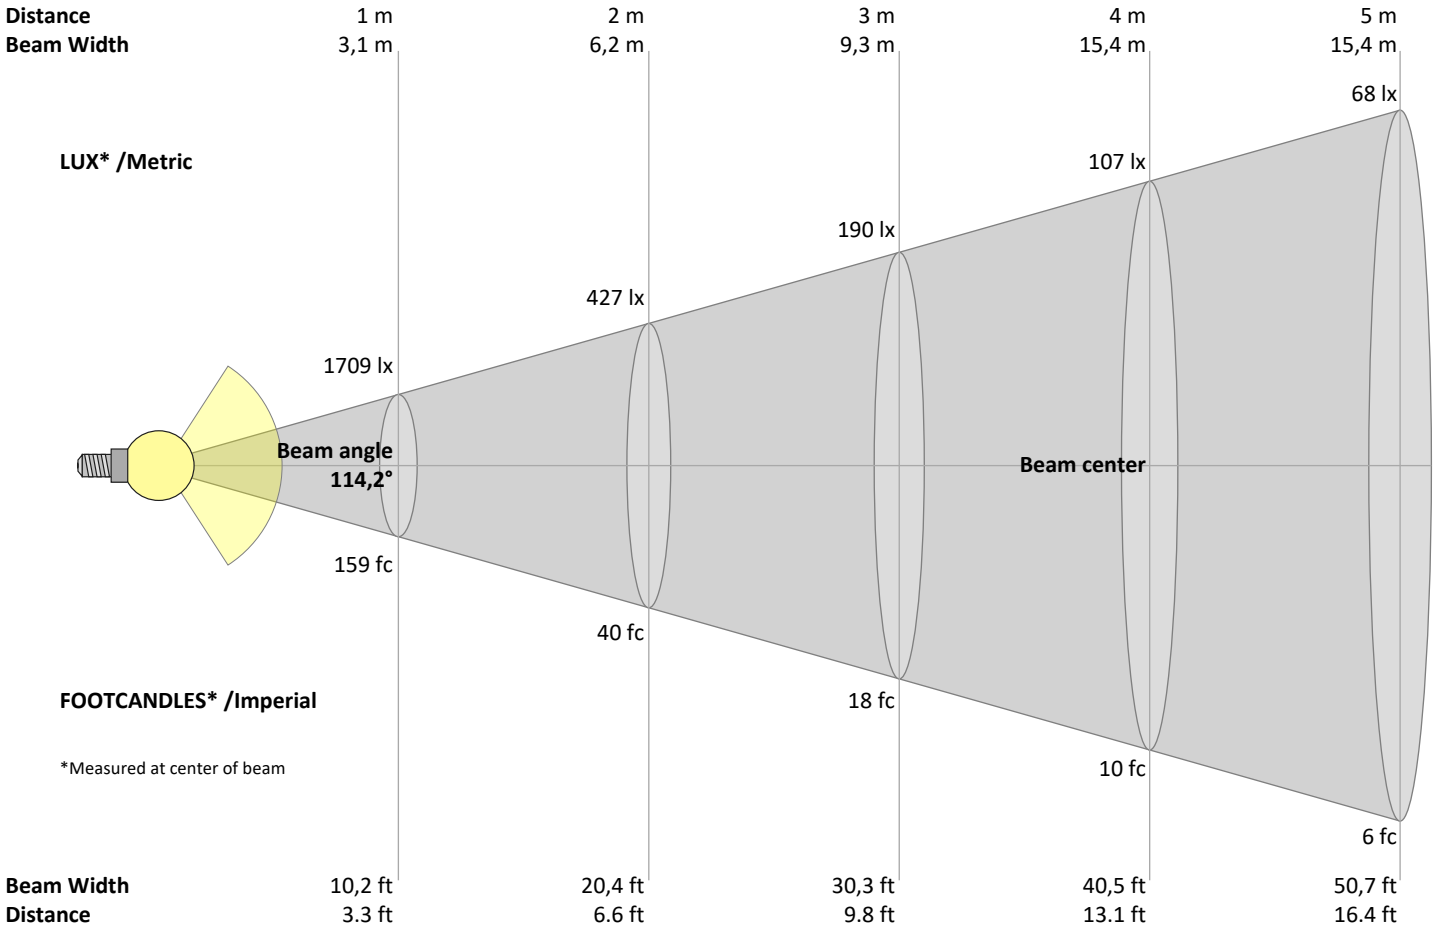

Beam intensities from 1 – 20 m

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	m
3,3	6,6	9,8	13,1	16,4	19,7	23	26,2	29,5	32,8	36,1	39,4	42,7	45,9	49,2	52,5	55,8	59,1	62,3	65,6	ft
1709	427	190	107	68	47	35	27	21	17	14	12	10	9	8	7	6	5	5	4	lux
158,8	39,7	17,6	9,9	6,4	4,4	3,2	2,5	2	1,6	1,3	1,1	0,9	0,8	0,7	0,6	0,5	0,5	0,4	0,4	fc

Intensities in 0° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
1709	1703	1681	1641	1588	1521	1441	1354	1253	1144	1028	906	782	659	538	423	319	230	160	109	cd
100%	100%	98%	96%	93%	89%	84%	79%	73%	67%	60%	53%	46%	39%	31%	25%	19%	13%	9%	6%	of 0°val

Intensities in 90° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
1709	1703	1681	1641	1588	1521	1441	1354	1253	1144	1028	906	782	659	538	423	319	230	160	109	cd
100%	100%	98%	96%	93%	89%	84%	79%	73%	67%	60%	53%	46%	39%	31%	25%	19%	13%	9%	6%	of 0°val

Intensities in 180° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
1709	1703	1681	1641	1588	1521	1441	1354	1253	1144	1028	906	782	659	538	423	319	230	160	109	cd
100%	100%	98%	96%	93%	89%	84%	79%	73%	67%	60%	53%	46%	39%	31%	25%	19%	13%	9%	6%	of 0°val

Intensities in 270° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
1709	1703	1681	1641	1588	1521	1441	1354	1253	1144	1028	906	782	659	538	423	319	230	160	109	cd
100%	100%	98%	96%	93%	89%	84%	79%	73%	67%	60%	53%	46%	39%	31%	25%	19%	13%	9%	6%	of 0°val

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)

Operator:



Light Planning – UGR table

Uncorrected, comprehensive UGR table according to 117-1995

Reflectances		70	70	50	50	30	70	70	50	50	30
	ρ Ceiling	70	70	50	50	30	70	70	50	50	30
	ρ Walls	50	30	50	30	30	50	30	50	30	30
	ρ Floor	20	20	20	20	20	20	20	20	20	20
Room size		Viewed Crosswise					Viewed Endwise				
H = mounting height above eye level		(Viewing direction orthogonal to lamp length axis)					(Viewing direction parallel to lamp length axis)				
X	Y										
2H	2H	22,1	23,3	22,4	23,7	24,0	22,4	23,6	22,7	24,0	24,3
	3H	23,7	25,0	24,2	25,3	25,6	24,1	25,3	24,5	25,7	26,0
	4H	24,5	25,7	25,0	26,1	26,4	24,9	26,1	25,4	26,5	26,8
	6H	25,3	26,3	25,6	26,7	27,1	25,8	26,9	26,2	27,2	27,7
	8H	25,6	26,6	26,0	27,0	27,5	26,2	27,3	26,6	27,6	28,1
	12H	25,9	26,9	26,3	27,3	27,8	26,6	27,7	27,1	28,0	28,6
4H	2H	22,8	24,0	23,2	24,3	24,7	23,0	24,2	23,4	24,5	24,9
	3H	24,7	25,7	25,1	26,1	26,6	25,0	26,0	25,4	26,4	26,9
	4H	25,5	26,5	26,1	27,0	27,6	25,9	26,9	26,4	27,3	28,0
	6H	26,4	27,3	27,0	27,7	28,2	26,9	27,8	27,5	28,2	28,7
	8H	26,8	27,6	27,4	28,1	28,5	27,4	28,2	28,0	28,7	29,1
	12H	27,2	27,9	27,7	28,4	28,9	27,9	28,6	28,5	29,1	29,7
8H	4H	25,9	26,8	26,5	27,2	27,7	26,3	27,1	26,8	27,5	28,0
	6H	27,0	27,7	27,6	28,2	28,8	27,5	28,1	28,0	28,6	29,3
	8H	27,6	28,1	28,1	28,7	29,4	28,1	28,7	28,7	29,3	30,0
	12H	28,1	28,6	28,7	29,1	29,8	28,8	29,3	29,4	29,9	30,5
12H	4H	26,0	26,7	26,6	27,2	27,7	26,3	27,0	26,9	27,5	28,0
	6H	27,2	27,7	27,8	28,3	29,0	27,6	28,2	28,2	28,7	29,5
	8H	27,8	28,3	28,4	28,8	29,5	28,3	28,8	28,9	29,3	30,0

Variations with the observer position for the luminaire spacings, S:

S = 1.0H	0,1 / -0,1	0,1 / -0,1
S = 1.5H	0,1 / -0,1	0,1 / -0,1
S = 2.0H	0,2 / -0,3	0,2 / -0,3

Coefficients of Utilization

Ceiling reflectance	80			70			50			30			10			0		
Wall reflectance	70	50	30	10	70	50	30	10	50	30	10	50	30	10	50	30	10	0
Floor reflectance	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	0
RCR	(RCR: Room Cavity Ratio) Room Values are expressed as percentage of Lumen delivered to the task surface																	
0	118	118	118	118	115	115	115	115	109	109	109	103	103	103	98	98	98	96
1	106	101	96	92	103	98	94	90	93	90	86	88	86	83	84	82	80	77
2	96	87	80	74	93	85	78	73	81	75	70	77	72	68	73	69	66	63
3	87	76	68	61	85	74	66	60	71	64	58	67	62	57	64	59	55	53
4	80	67	58	51	77	66	57	51	63	55	50	60	53	48	57	52	47	45
5	73	60	51	44	71	59	50	44	56	48	43	54	47	42	51	46	41	39
6	68	54	45	38	66	53	44	38	51	43	37	48	42	37	46	41	36	34
7	63	49	40	34	61	48	39	33	46	38	33	44	37	32	42	36	32	30
8	58	45	36	30	57	44	36	30	42	35	29	40	34	29	39	33	28	26
9	55	41	33	27	53	40	32	27	39	31	26	37	31	26	36	30	26	24
10	51	38	30	24	50	37	29	24	36	29	24	35	28	24	33	28	23	22

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)


Operator:



Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

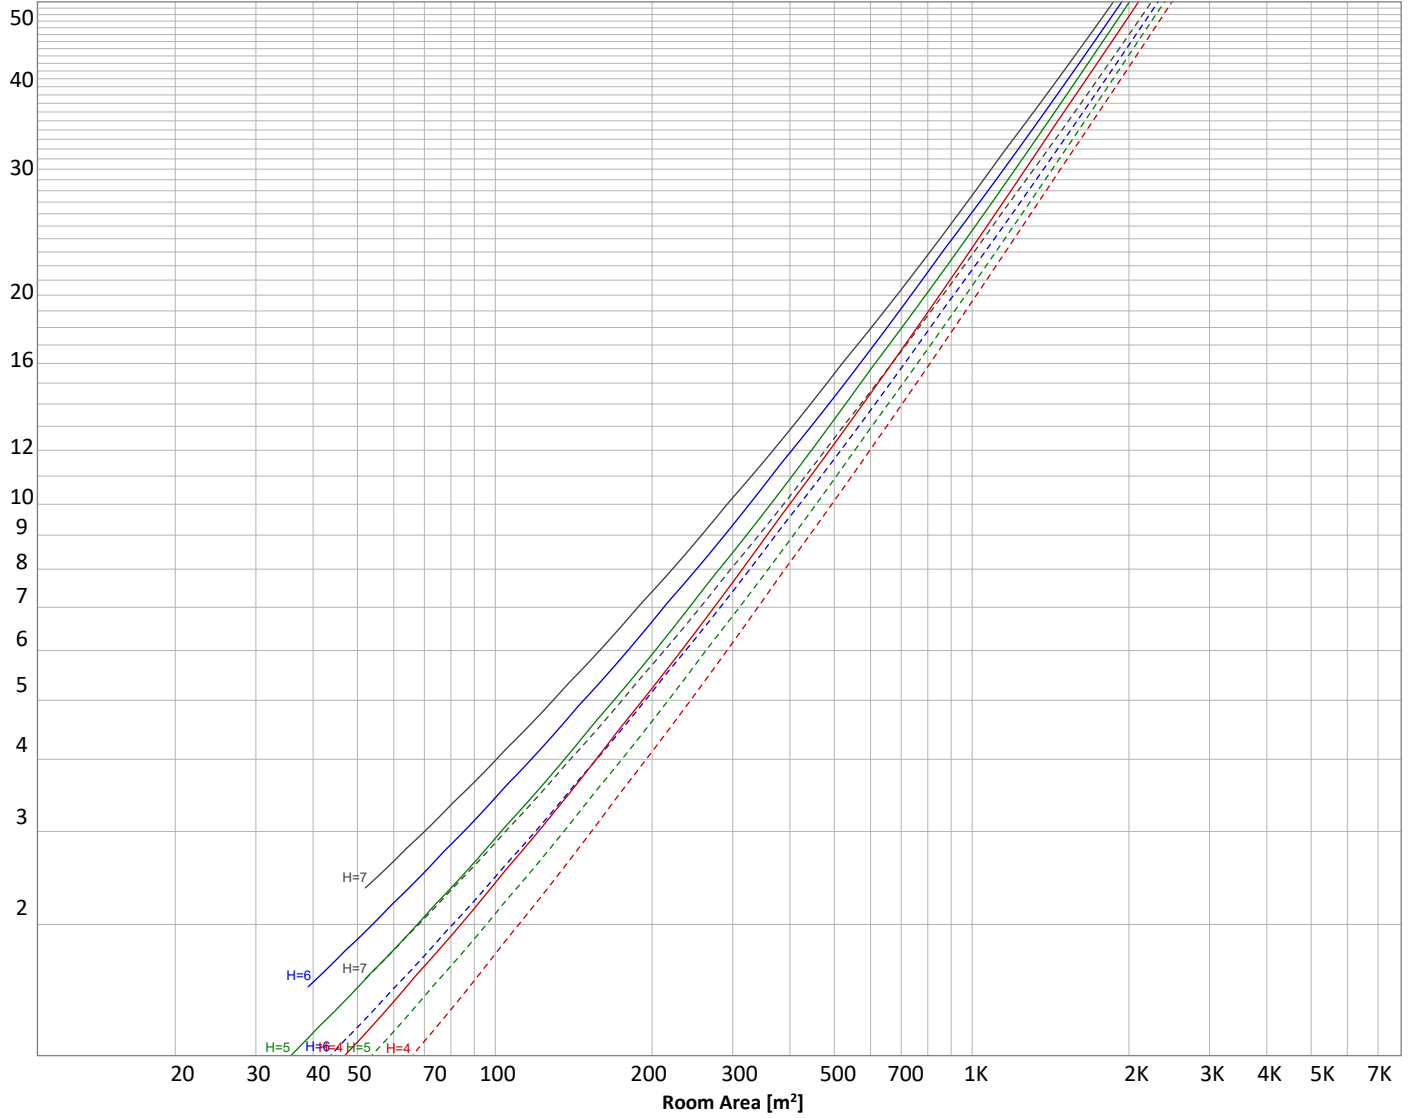

Conditions

H = Room height	Flux = 5458 lm				
H _{down} = Lamp distance from ceiling =	0.00 m	Line type	Ceiling reflectance	ρ(%) Wall reflectance	Floor reflectance
H _{work} = Work area height from floor =	0.00 m	-----	70	50	30
E _{work} = Average lux on work area =	100 lx	—————	50	30	20

Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
162 lm	463 lm	700 lm	846 lm	882 lm	810 lm	653 lm	449 lm	255 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
122 lm	50,5 lm	19,4 lm	11,4 lm	10,5 lm	9,55 lm	7,78 lm	5,31 lm	2,00 lm

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](#)

Operator:



Outdoor Light Planning

Lumen per Zone

Zone (γ)	Lumen	% Total
0-10°	162 lm	3,0%
10-20°	463 lm	8,5%
20-30°	700 lm	12,8%
30-40°	846 lm	15,5%
40-50°	882 lm	16,2%
50-60°	810 lm	14,8%
60-70°	653 lm	12,0%
70-80°	449 lm	8,2%
80-90°	255 lm	4,7%
90-100°	122 lm	2,2%
100-110°	51 lm	0,9%
110-120°	19 lm	0,4%
120-130°	11 lm	0,2%
130-140°	10 lm	0,2%
140-150°	10 lm	0,2%
150-160°	8 lm	0,1%
160-170°	5 lm	0,1%
170-180°	2 lm	0,0%
Total	5458 lm	100,0%

Intensity peaks

Max intensity	1709 cd
Intensity, 90°	160 cd
Intensity, 0°	1709 cd

Zonal Lumen summary


Zone (γ)	Lumen	% Total
0-30°	1325 lm	24,3%
0-40°	2170 lm	39,8%
0-60°	3862 lm	70,8%
60-90°	1357 lm	24,9%
70-100°	827 lm	15,1%
90-120°	192 lm	3,5%
0-90°	5219 lm	95,6%
90-180°	239 lm	4,4%
0-180°	5458 lm	100,0%

BUG rating

	Lumen	% Total
Forward light		
Low(0-30°)	662 lm	12,1%
Medium(30-60°)	1269 lm	23,2%
High(60-80°)	551 lm	10,1%
Very high(80-90°)	128 lm	2,3%
Back light		
Low(0-30°)	662 lm	12,1%
Medium(30-60°)	1269 lm	23,2%
High(60-80°)	551 lm	10,1%
Very high(80-90°)	128 lm	2,3%
Uplight		
Low(90-100°)	122 lm	2,2%
High(100-180°)	117 lm	2,1%

IESNA TM-15-07 Luminaire Classification System For Outdoor Luminaires

BUG rating B2 U3 G2

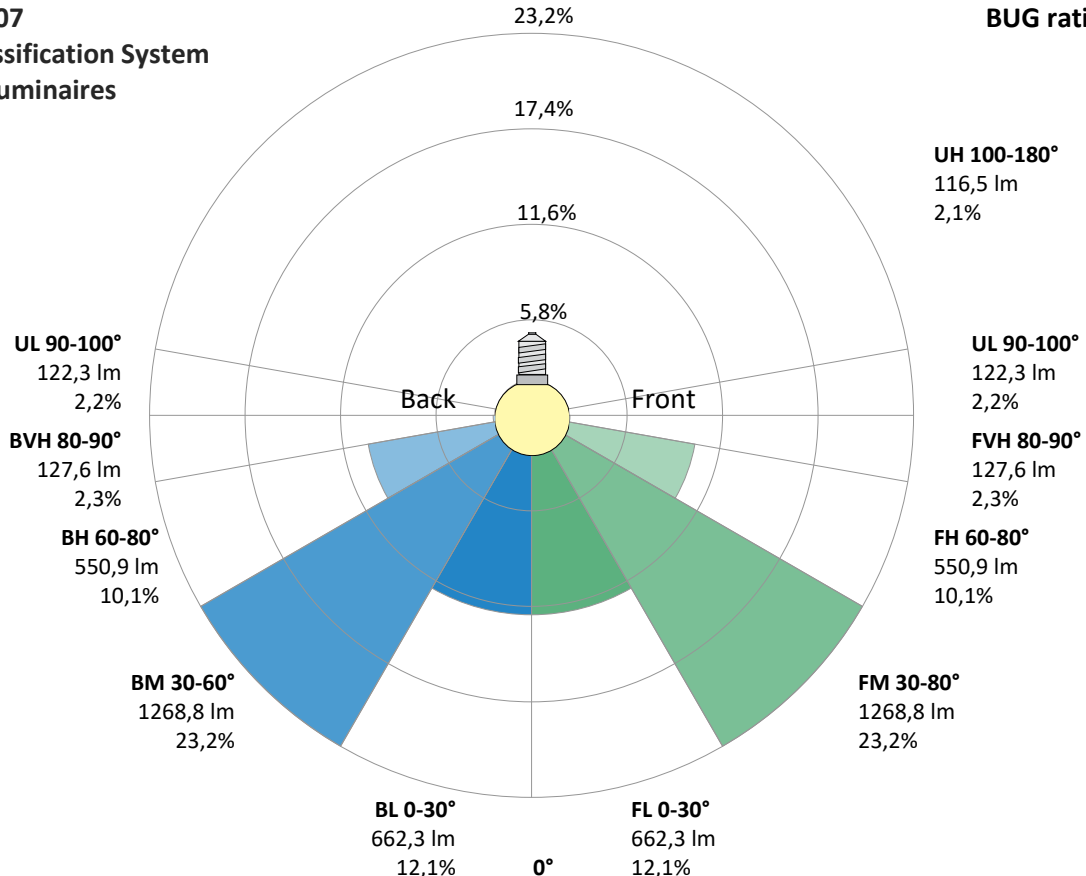

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](#)

Operator:




Power Details

Input Power

Power feed to light source	49,9 W
Frequency of input power	50 Hz
RMS Input voltage feed, V_{RMS}	230 V
RMS Input current feed, I_{RMS}	0,222 A
Volt-Ampere or apparent power = $V_{RMS} * I_{RMS}$	51,05 VA
Displacement factor of AC power feed	0,98
Power factor of AC current feed	0,98
Total harmonic distortion of the current	9,02%
Total harmonic distortion of the voltage	0,07%

Input Power Curve

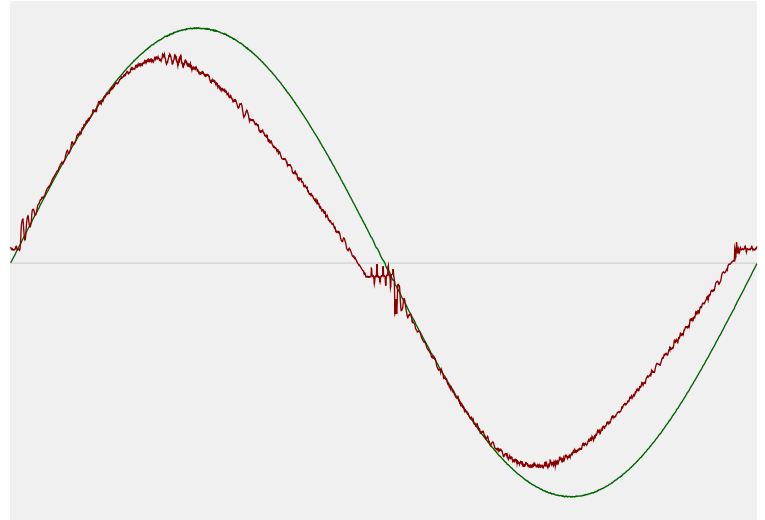

Efficiency

Radiated power efficiency 34,8%



Lumen efficiency 109 lm/W



Stabilization Details

Warmup Conditions

Stable period	15 min
Stable change max	2,0%
Minimum time	15 min

Color Temperature Change

CCT start	2986 K
CCT shift	+14 K
CCT end	3000 K


Warmup Result

Total warmup time	Lamp stabilized in 15 min 1 sec
Warmup variation	-1,0%

Output Change

Output start	5512 lm
Output change	-54 lm
Output end	5458 lm

Stabilization Curve

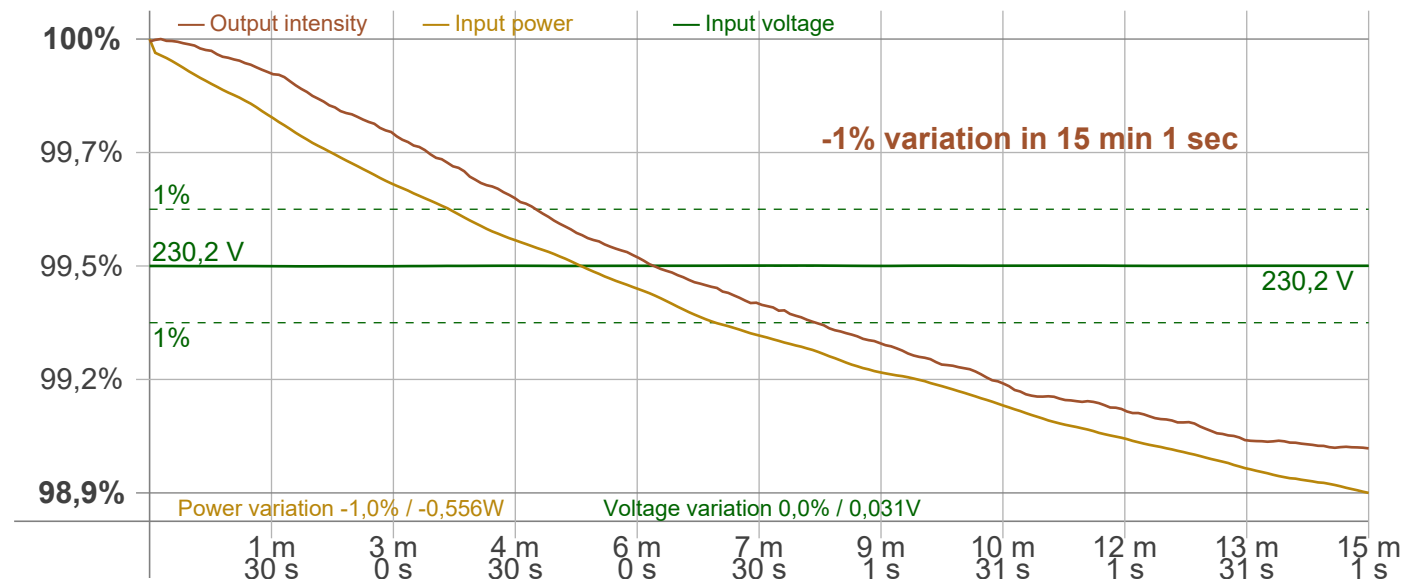

Light Measurement Report

Print date: 8-9-2025

Measurement date and time: 8-9-2025 15:20:10 – Measurement no. VFR-250908-3037-MS

Measurement tracking No. and Link: [VT250908-000895](https://www.viso-systems.com/VT250908-000895)

Operator:



Flicker /TLA details

Flicker Meter Type Viso Systems LabFlicker
 Frequency of input power 50 Hz
 Flicker/TLA sample rate 20000 samples/s

Measurement time
 PstLM 180 sec
 All other indices 1,2 sec

Flicker indices according to Illuminating Engineering Society (IES)

Flicker frequency 100 Hz
 Percent Flicker 0,29 %
 Flicker index 0

Flicker indices according to California Energy Commission (CEC) 2016b

JA8/10 40 Hz 0,01 %
 JA8/10 90 Hz 0,02 %
 JA8/10 200 Hz 0,27 %
 JA8/10 400 Hz 0,27 %
 JA8/10 1000 Hz 0,28 %


TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)

PstLM value (F < 80 Hz) 0,01
 SVM value (80 < F < 2000 Hz) 0,01

Flicker indices according to Lighting Research Center (2015)

Perception metric, Assist Mp 0

Flicker frame (frame of one flicker period in time domain)

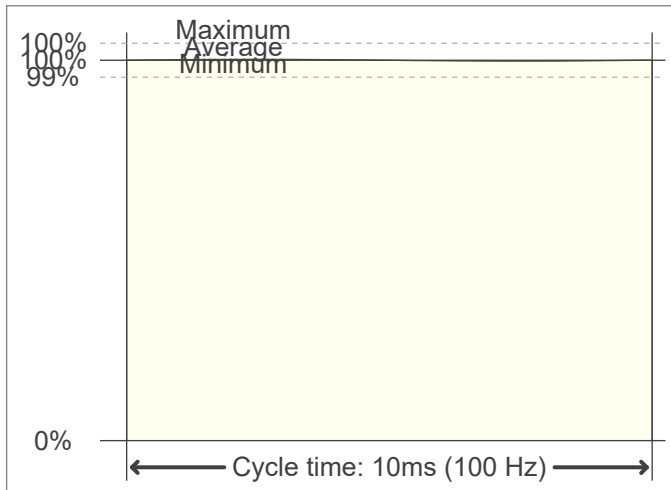

Flicker FFT (flicker curve in frequency domain)



IEEE 1789 Frequency/modulation plot

